

LB 109649

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Dk

Instrument ID : Konelab

6/18/2020 13:41

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.248	0.0	0.082	
ICB1	-0.264	0.0	0.004	
CCV1	240.801	0.0	0.198	
CCB1	-0.173	0.0	0.004	
PB129615BL	-0.465	0.0	0.003	
L2809-04	-0.233	0.0	0.004	
L2809-04DUP	-0.154	0.0	0.004	
L2812-10	-0.635	0.0	0.003	
L2813-12	-0.676	0.0	0.003	
L2817-10	-0.706	0.0	0.003	
L3048-01	-0.751	0.0	0.003	
PB129616BL	-0.574	0.0	0.003	
L3048-02	-0.587	0.0	0.003	
CCV2	247.587	0.0	0.203	
CCB2	-0.330	0.0	0.004	
L3048-02DUP	-0.438	0.0	0.003	
L2818-04	-0.604	0.0	0.003	
L2818-04	-0.217	0.0	0.004	
CCV3	254.286	0.0	0.209	
CCB3	-0.351	0.0	0.003	

N 20
Mean 41.638
SD 91.4019
CV% 219.51

L2815-10

Dk
06/18/2020

Aquakem v. 7.2AQ1

Results from time period:

Thu Jun 18 12:03:54 2020

Thu Jun 18 13:36:28 2020



Sample Id	Sam/Ctr/c/	Test short narr	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	REACTIVE CN	P	-0.804	µg/l	6/18/2020 12:03:54	
5.OPPBCN	A	REACTIVE CN	P	4.0758	µg/l	6/18/2020 12:03:55	
10PPBCN	A	REACTIVE CN	P	9.8996	µg/l	6/18/2020 12:03:56	
50PPBCN	A	REACTIVE CN	P	50.7029	µg/l	6/18/2020 12:03:57	
100PPBCN	A	REACTIVE CN	P	102.1885	µg/l	6/18/2020 12:03:58	
250PPBCN	A	REACTIVE CN	P	248.8678	µg/l	6/18/2020 12:03:59	
500PPBCN	A	REACTIVE CN	P	500.0694	µg/l	6/18/2020 12:04:00	
ICV1	S	REACTIVE CN	P	97.2478	µg/l	6/18/2020 12:47:54	
ICB1	S	REACTIVE CN	P	-0.2643	µg/l	6/18/2020 12:47:55	
CCV1	S	REACTIVE CN	P	240.8006	µg/l	6/18/2020 12:47:56	
CCB1	S	REACTIVE CN	P	-0.1732	µg/l	6/18/2020 12:47:57	
PB129615E	S	REACTIVE CN	P	-0.4648	µg/l	6/18/2020 12:47:58	
L2809-04	S	REACTIVE CN	P	-0.2333	µg/l	6/18/2020 12:47:59	
L2809-04D	S	REACTIVE CN	P	-0.1536	µg/l	6/18/2020 12:48:00	
L2812-10	S	REACTIVE CN	P	-0.6347	µg/l	6/18/2020 12:48:01	
L2813-12	S	REACTIVE CN	P	-0.6757	µg/l	6/18/2020 12:48:02	
L2817-10	S	REACTIVE CN	P	-0.7058	µg/l	6/18/2020 12:48:03	
L3048-01	S	REACTIVE CN	P	-0.7514	µg/l	6/18/2020 12:54:05	
PB129616E	S	REACTIVE CN	P	-0.5743	µg/l	6/18/2020 12:54:06	
L3048-02	S	REACTIVE CN	P	-0.5867	µg/l	6/18/2020 12:54:07	
CCV2	S	REACTIVE CN	P	247.5875	µg/l	6/18/2020 12:54:08	
CCB2	S	REACTIVE CN	P	-0.3304	µg/l	6/18/2020 12:54:09	
L3048-02D	S	REACTIVE CN	P	-0.4379	µg/l	6/18/2020 12:54:10	
L2818-04	S	REACTIVE CN	P	-0.6038	µg/l	6/18/2020 13:16:57	
L2815-10	S	REACTIVE CN	P	-0.2174	µg/l	6/18/2020 13:16:58	
CCV3	S	REACTIVE CN	P	254.2857	µg/l	6/18/2020 13:36:26	
CCB3	S	REACTIVE CN	P	-0.3509	µg/l	6/18/2020 13:36:27	

LB109649

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Du

Instrument ID : Konelab

6/18/2020 12:06


Test ^{Reche}
~~Total~~ CN

Accepted 6/18/2020 12:06

Factor 1240
Bias 0.004

Coeff. of det. 0.999961

Errors

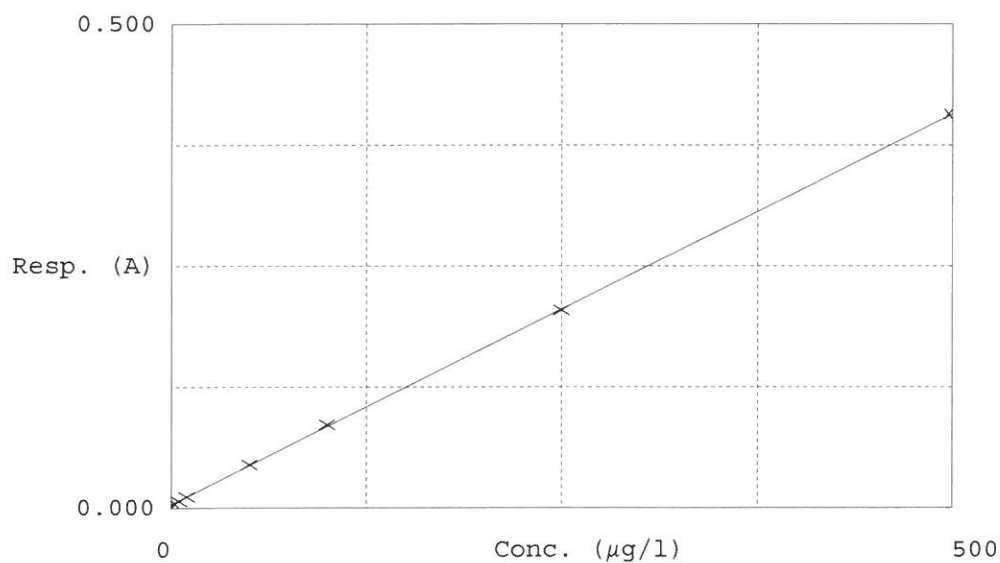

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.8040	0.0000	
2	5.0PPBCN	0.007	4.0758	5.0000	
3	10PPBCN	0.012	9.8996	10.0000	
4	50PPBCN	0.045	50.7029	50.0000	
5	100PPBCN	0.086	102.1885	100.0000	
6	250PPBCN	0.204	248.8678	250.0000	
7	500PPBCN	0.407	500.0694	500.0000	