


L3109696

7470A

INSTRUMENT ID: CV1

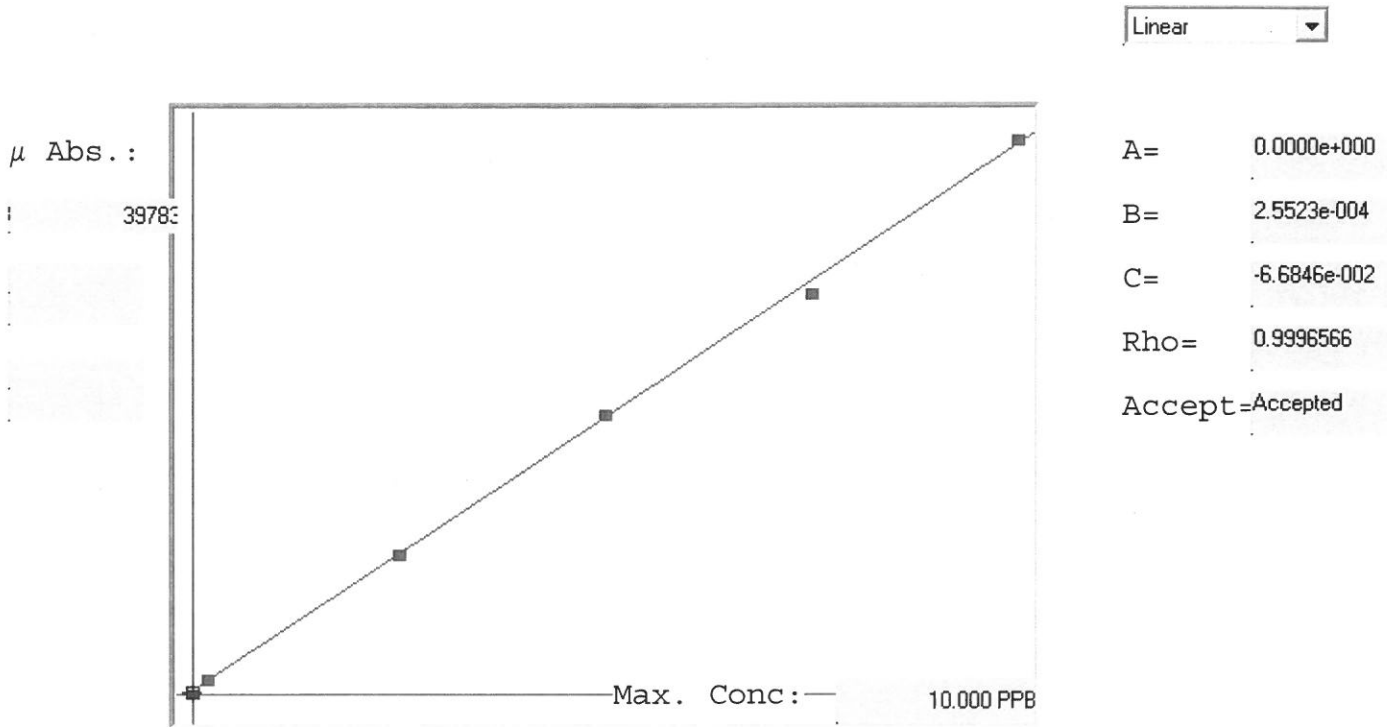

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.030	-0.030	145	0.000	145				
0.2	0.200	0.216	0.016	1109	0.0 %	1109				
2.5	2.500	2.530	0.030	10175	0.0 %	10175				
5.0	5.000	5.091	0.091	20210	0.0 %	20210				
7.5	7.500	7.305	-0.195	28882	0.0 %	28882				
10.0	10.000	10.087	0.087	39783	0.0 %	39783				

LB109696 INSTRUMENT ID : CV1

Method: 7470A	Operator: Admin	Date of Analysis: 23 Jun 2020 10:20:14							
Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	145	-	0.0000	7470A	PPB	23 Jun 2020 10:28:02	S	Std
0.2 - 1	50.2	1109	-	0.2000	7470A	PPB	23 Jun 2020 10:30:10	S	Std
2.5 - 1	52.5	10175	-	2.5000	7470A	PPB	23 Jun 2020 10:32:17	S	Std
5.0 - 1	55	20210	-	5.0000	7470A	PPB	23 Jun 2020 10:34:25	S	Std
7.5 - 1	57.5	28882	-	7.5000	7470A	PPB	23 Jun 2020 10:39:02	S	Std
10.0 - 1	510	39783	-	10.0000	7470A	PPB	23 Jun 2020 10:46:03	S	Std
ICV94 - 1	ICV94	15950	4.0041	-	7470A	PPB	23 Jun 2020 10:48:36	U	SMPL
ICB94 - 1	ICB94	208	-0.0138	-	7470A	PPB	23 Jun 2020 10:50:42	U	SMPL
CCV61 - 1	CCV61	20228	5.0960	-	7470A	PPB	23 Jun 2020 10:52:48	U	SMPL
CCB61 - 1	CCB61	210	-0.0132	-	7470A	PPB	23 Jun 2020 10:54:54	U	SMPL
CRA - 1	CRA	1196	0.2384	-	7470A	PPB	23 Jun 2020 10:57:00	U	SMPL
HighStd - 1	HighStd	39431	9.9973	-	7470A	PPB	23 Jun 2020 10:59:05	U	SMPL
ChkStd - 1	ChkStd	26852	6.7867	-	7470A	PPB	23 Jun 2020 11:01:12	U	SMPL
PB129681BL - 1	PBW	259	-0.0007	-	7470A	PPB	23 Jun 2020 11:03:19	U	SMPL
PB129681BS - 1	LCSW	16067	4.0340	-	7470A	PPB	23 Jun 2020 11:05:27	U	SMPL
L3051-02 - 1	SLUDGE-BOX	237	-0.0064	-	7470A	PPB	23 Jun 2020 11:07:34	U	SMPL
L3051-02DUP - 1	SLUDGE-BOXDUP	283	0.0054	-	7470A	PPB	23 Jun 2020 11:09:41	U	SMPL
L3051-02MS - 1	SLUDGE-BOXMS	16522	4.1501	-	7470A	PPB	23 Jun 2020 11:11:48	U	SMPL
L3051-02MSD - 1	SLUDGE-BOXMSD	16857	4.2356	-	7470A	PPB	23 Jun 2020 11:13:56	U	SMPL
L3081-01 - 1	JFK-WC-S-SB-01	288	0.0067	-	7470A	PPB	23 Jun 2020 11:16:02	U	SMPL
CCV62 - 1	CCV62	20464	5.1563	-	7470A	PPB	23 Jun 2020 11:18:07	U	SMPL
CCB62 - 1	CCB62	243	-0.0048	-	7470A	PPB	23 Jun 2020 11:20:14	U	SMPL
PB129682BL - 1	PBW	324	0.0158	-	7470A	PPB	23 Jun 2020 11:22:20	U	SMPL
PB129682BS - 1	LCSW	15854	3.9796	-	7470A	PPB	23 Jun 2020 11:24:27	U	SMPL
L3080-01 - 1	JFK-GW-01-15	416	0.0393	-	7470A	PPB	23 Jun 2020 11:26:34	U	SMPL
L3080-01DUP - 1	JFK-GW-01-15DUP	481	0.0559	-	7470A	PPB	23 Jun 2020 11:28:41	U	SMPL
L3080-01MS - 1	JFK-GW-01-15MS	16977	4.2663	-	7470A	PPB	23 Jun 2020 11:30:47	U	SMPL
L3080-01MSD - 1	JFK-GW-01-15MSD	16900	4.2466	-	7470A	PPB	23 Jun 2020 11:32:54	U	SMPL
L3080-02 - 1	JFK-GW-01-15-D	487	0.0575	-	7470A	PPB	23 Jun 2020 11:35:01	U	SMPL
L3081-02 - 1	JFK-WC-L-01	465	0.0518	-	7470A	PPB	23 Jun 2020 11:37:09	U	SMPL
CCV63 - 1	CCV63	20153	5.0769	-	7470A	PPB	23 Jun 2020 11:39:17	U	SMPL
CCB63 - 1	CCB63	256	-0.0015	-	7470A	PPB	23 Jun 2020 11:41:23	U	SMPL
PB129681TB - 1	PB129654TB	293	0.0079	-	7470A	PPB	23 Jun 2020 11:43:29	U	SMPL
L3051-02LX5 - 1		191	-0.0181	-	7470A	PPB	23 Jun 2020 11:45:36	U	SMPL
L3051-02A - 1		16109	4.0447	-	7470A	PPB	23 Jun 2020 11:47:42	U	SMPL
L3080-01LX5 - 1		141	-0.0309	-	7470A	PPB	23 Jun 2020 11:49:48	U	SMPL
L3080-01A - 1		16834	4.2298	-	7470A	PPB	23 Jun 2020 11:51:54	U	SMPL
CCV64 - 1	CCV64	19778	4.9812	-	7470A	PPB	23 Jun 2020 11:54:01	U	SMPL
CCB64 - 1	CCB64	245	-0.0043	-	7470A	PPB	23 Jun 2020 11:56:07	U	SMPL