


LB109717

7471B

INSTRUMENT ID: CVJ

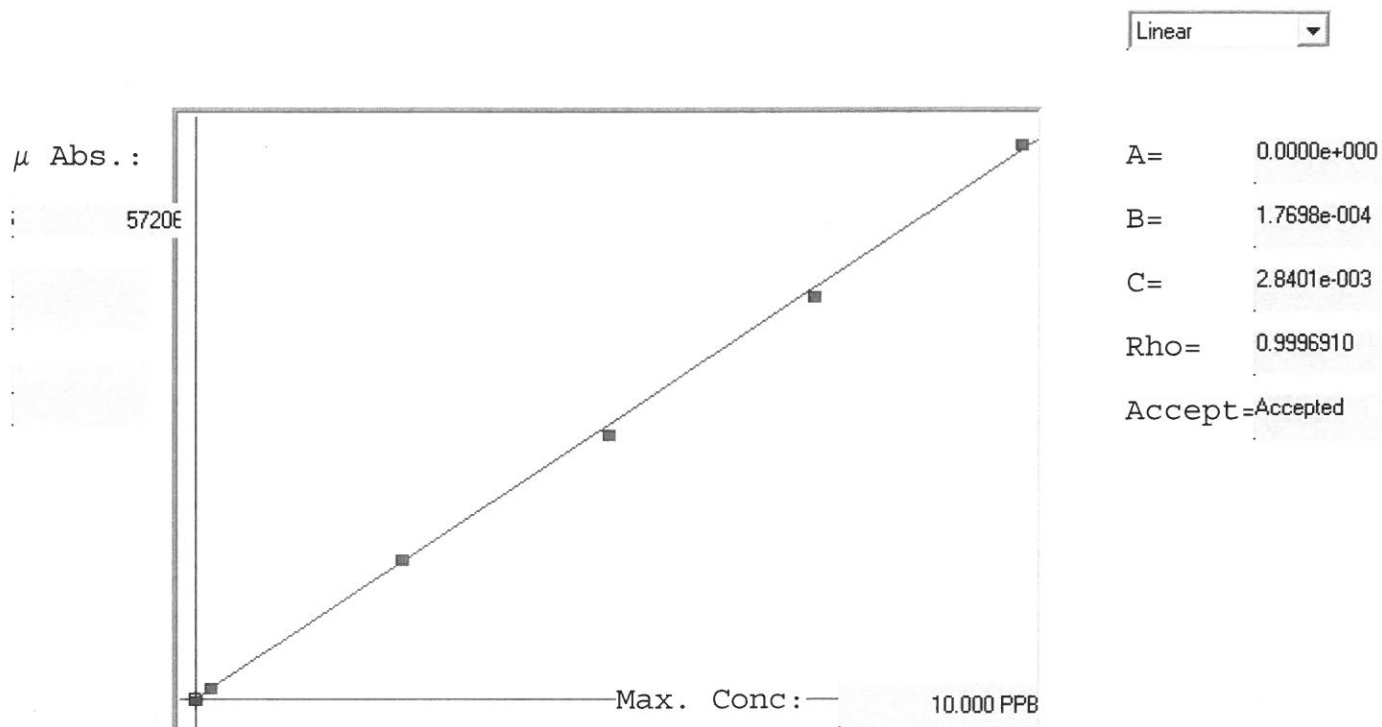

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.035	0.035	184	0.000	184				
0.2	0.200	0.216	0.016	1203	0.0 %	1203				
2.5	2.500	2.562	0.062	14458	0.0 %	14458				
5.0	5.000	4.872	-0.128	27512	0.0 %	27512				
7.5	7.500	7.388	-0.112	41727	0.0 %	41727				
10.0	10.000	10.127	0.127	57206	0.0 %	57206				

LB109717 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 24 Jun 2020 13:46:00

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	184	-	0.00007471B		PPB	24 Jun 2020 13:48:46	S	Std
0.2 - 1	50.2	1203	-	0.20007471B		PPB	24 Jun 2020 13:51:04	S	Std
2.5 - 1	52.5	14458	-	2.50007471B		PPB	24 Jun 2020 13:53:21	S	Std
5.0 - 1	55	27512	-	5.00007471B		PPB	24 Jun 2020 13:55:37	S	Std
7.5 - 1	57.5	41727	-	7.50007471B		PPB	24 Jun 2020 14:00:43	S	Std
10.0 - 1	50	57206	-	10.00007471B		PPB	24 Jun 2020 14:05:37	S	Std
ICV97 - 1	ICV97	22515	3.9876	-7471B		PPB	24 Jun 2020 14:08:27	U	SMPL
ICB97 - 1	ICB97	-96	-0.0142	-7471B		PPB	24 Jun 2020 14:10:41	U	SMPL
CCV72 - 1	CCV72	27400	4.8522	-7471B		PPB	24 Jun 2020 14:12:57	U	SMPL
CCB72 - 1	CCB72	-114	-0.0173	-7471B		PPB	24 Jun 2020 14:15:13	U	SMPL
CRA - 1	CRA	1194	0.2142	-7471B		PPB	24 Jun 2020 14:17:28	U	SMPL
HighStd - 1	HighStd	58011	10.2698	-7471B		PPB	24 Jun 2020 14:19:43	U	SMPL
ChkStd - 1	ChkStd	40995	7.2583	-7471B		PPB	24 Jun 2020 14:21:58	U	SMPL
PB129727BL - 1	PBS	-217	-0.0356	-7471B		PPB	24 Jun 2020 14:24:16	U	SMPL
PB129727BS - 1	LCSS	20186	3.5754	-7471B		PPB	24 Jun 2020 14:26:33	U	SMPL
L2818-07 - 1	TR-05-062320	5172	0.9182	-7471B		PPB	24 Jun 2020 14:28:49	U	SMPL
L3086-01 - 1	363	765	0.1382	-7471B		PPB	24 Jun 2020 14:31:06	U	SMPL
L3089-01 - 1	RB47184-RT	5972	1.0598	-7471B		PPB	24 Jun 2020 14:33:23	U	SMPL
L3089-04 - 1	RB44767-RT	4736	0.8410	-7471B		PPB	24 Jun 2020 14:35:40	U	SMPL
L3089-07 - 1	RB47185-RT	4927	0.8748	-7471B		PPB	24 Jun 2020 14:37:55	U	SMPL
CCV73 - 1	CCV73	27531	4.8754	-7471B		PPB	24 Jun 2020 14:40:10	U	SMPL
CCB73 - 1	CCB73	-111	-0.0168	-7471B		PPB	24 Jun 2020 14:42:26	U	SMPL
L3090-01 - 1	359-RO	1555	0.2780	-7471B		PPB	24 Jun 2020 14:44:42	U	SMPL
L3094-01 - 1	BRENNAN-FL-001	109	0.0221	-7471B		PPB	24 Jun 2020 14:46:58	U	SMPL
L3094-02 - 1	2020-06-22-FD04	113	0.0228	-7471B		PPB	24 Jun 2020 14:49:13	U	SMPL
L3096-01 - 1	FK-GF-03-011-A	7092	1.2580	-7471B		PPB	24 Jun 2020 14:51:29	U	SMPL
L3096-03 - 1	FK-GF-03-011-B	9029	1.6008	-7471B		PPB	24 Jun 2020 14:58:34	U	SMPL
L3096-03DUP - 1	FK-GF-03-011-BDUP	8952	1.5872	-7471B		PPB	24 Jun 2020 15:00:50	U	SMPL
L3096-03MS - 1	FK-GF-03-011-BMS	28606	5.0656	-7471B		PPB	24 Jun 2020 15:03:06	U	SMPL
L3096-03MSD - 1	FK-GF-03-011-BMSD	28406	5.0302	-7471B		PPB	24 Jun 2020 15:05:23	U	SMPL
L3096-03LX5 - 1		1908	0.3405	-7471B		PPB	24 Jun 2020 15:07:40	U	SMPL
L3096-03A - 1		32114	5.6865	-7471B		PPB	24 Jun 2020 15:09:55	U	SMPL
CCV74 - 1	CCV74	27439	4.8591	-7471B		PPB	24 Jun 2020 15:12:11	U	SMPL
CCB74 - 1	CCB74	-101	-0.0150	-7471B		PPB	24 Jun 2020 15:14:27	U	SMPL