


LB109726

7470A

INSTRUMENT ID: CV2

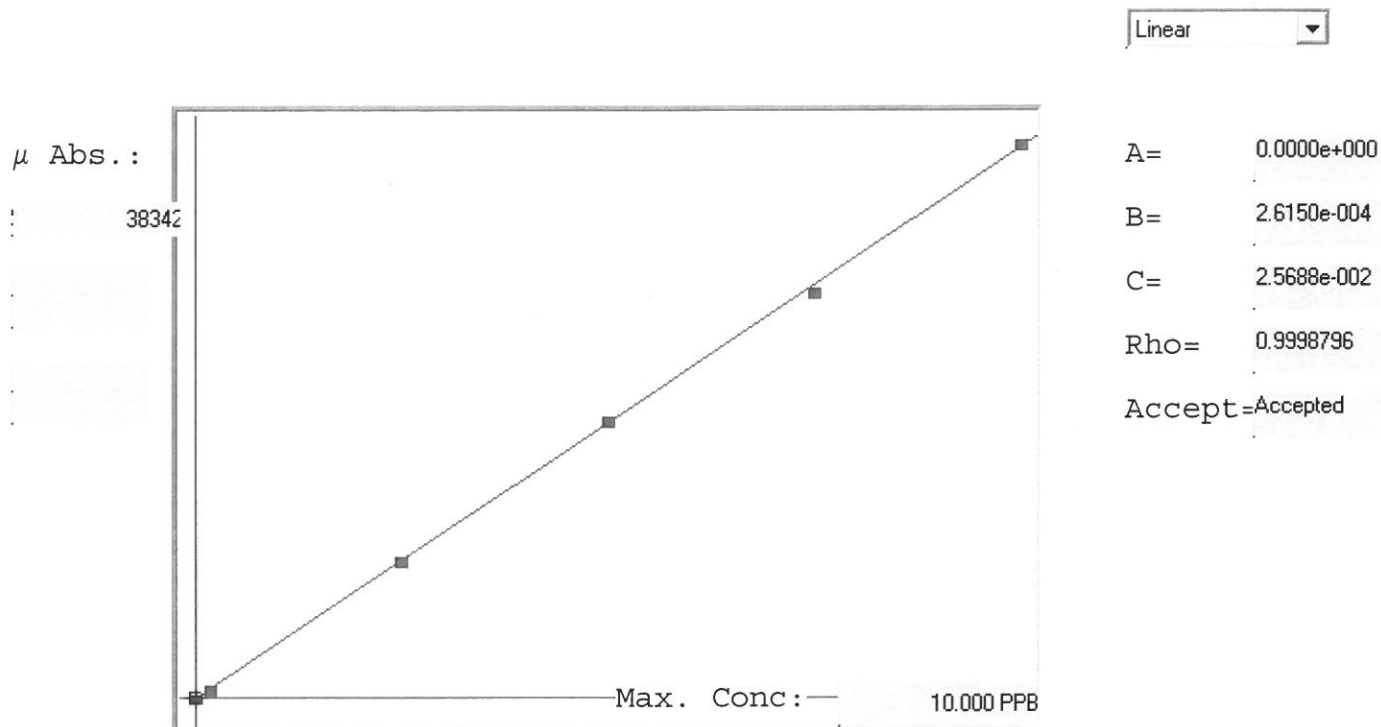

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	-123	0.000	-123				
0.2	0.200	0.198	-0.002	658	0.0 %	658				
2.5	2.500	2.514	0.014	9515	0.0 %	9515				
5.0	5.000	5.058	0.058	19245	0.0 %	19245				
7.5	7.500	7.385	-0.115	28141	0.0 %	28141				
10.0	10.000	10.052	0.052	38342	0.0 %	38342				

LB109726 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 25 Jun 2020 09:13:54					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-123	-	0.00007470A	PPB		25 Jun 2020 10:31:57	S	Std
0.2 - 1	50.2	658	-	0.20007470A	PPB		25 Jun 2020 10:34:04	S	Std
2.5 - 1	52.5	9515	-	2.50007470A	PPB		25 Jun 2020 10:36:13	S	Std
5.0 - 1	55	19245	-	5.00007470A	PPB		25 Jun 2020 10:38:20	S	Std
7.5 - 1	57.5	28141	-	7.50007470A	PPB		25 Jun 2020 10:40:27	S	Std
10.0 - 1	510	38342	-	10.00007470A	PPB		25 Jun 2020 10:42:33	S	Std
ICV98 - 1	ICV98	14519	3.8224	-7470A	PPB		25 Jun 2020 10:45:13	U	SMPL
ICB98 - 1	ICB98	-98	0.0001	-7470A	PPB		25 Jun 2020 10:47:19	U	SMPL
CCV75 - 1	CCV75	18745	4.9275	-7470A	PPB		25 Jun 2020 10:52:51	U	SMPL
CCB75 - 1	CCB75	-88	0.0027	-7470A	PPB		25 Jun 2020 10:54:56	U	SMPL
CRA - 1	CRA	650	0.1957	-7470A	PPB		25 Jun 2020 10:57:02	U	SMPL
HighStd - 1	HighStd	38524	10.0997	-7470A	PPB		25 Jun 2020 10:59:08	U	SMPL
ChkStd - 1	ChkStd	27006	7.0877	-7470A	PPB		25 Jun 2020 11:01:14	U	SMPL
PB129743BL - 1	PBW	-143	-0.0117	-7470A	PPB		25 Jun 2020 11:03:22	U	SMPL
PB129743BS - 1	LCSW	13747	3.6205	-7470A	PPB		25 Jun 2020 11:05:29	U	SMPL
L3094-03 - 1	BRENNAN-FL-001	-68	0.0079	-7470A	PPB		25 Jun 2020 11:14:42	U	SMPL
L3094-03DUP - 1	BRENNAN-FL-001DUP	-82	0.0042	-7470A	PPB		25 Jun 2020 11:16:48	U	SMPL
L3094-03MS - 1	BRENNAN-FL-001MS	13656	3.5967	-7470A	PPB		25 Jun 2020 11:18:56	U	SMPL
L3094-03MSD - 1	BRENNAN-FL-001MSD	13501	3.5562	-7470A	PPB		25 Jun 2020 11:21:04	U	SMPL
L3094-04 - 1	2020-06-22-FD04	-127	-0.0075	-7470A	PPB		25 Jun 2020 11:23:10	U	SMPL
CCV76 - 1	CCV76	19680	5.1720	-7470A	PPB		25 Jun 2020 11:25:16	U	SMPL
CCB76 - 1	CCB76	-55	0.0113	-7470A	PPB		25 Jun 2020 11:27:22	U	SMPL
PB129744BL - 1	PBW	-14	0.0220	-7470A	PPB		25 Jun 2020 11:29:28	U	SMPL
PB129744BS - 1	LCSW	14616	3.8478	-7470A	PPB		25 Jun 2020 11:31:34	U	SMPL
L2818-10 - 1	TR-05-062320	-39	0.0155	-7470A	PPB		25 Jun 2020 11:33:41	U	SMPL
L3086-02 - 1	363	-10	0.0231	-7470A	PPB		25 Jun 2020 11:35:47	U	SMPL
L3089-02 - 1	RB47184-RT	-4	0.0246	-7470A	PPB		25 Jun 2020 11:37:54	U	SMPL
L3089-05 - 1	RB44767-RT	-9	0.0233	-7470A	PPB		25 Jun 2020 11:40:01	U	SMPL
L3089-08 - 1	RB47185-RT	-4	0.0246	-7470A	PPB		25 Jun 2020 11:42:09	U	SMPL
L3089-08DUP - 1	RB47185-RTDUP	-2	0.0252	-7470A	PPB		25 Jun 2020 11:44:16	U	SMPL
L3089-08MS - 1	RB47185-RTMS	14507	3.8193	-7470A	PPB		25 Jun 2020 11:46:25	U	SMPL
L3089-08MSD - 1	RB47185-RTMSD	14365	3.7821	-7470A	PPB		25 Jun 2020 11:48:31	U	SMPL
CCV77 - 1	CCV77	19831	5.2115	-7470A	PPB		25 Jun 2020 11:50:38	U	SMPL
CCB77 - 1	CCB77	-70	0.0074	-7470A	PPB		25 Jun 2020 11:52:44	U	SMPL
PB129745BL - 1	PBW	-14	0.0220	-7470A	PPB		25 Jun 2020 11:54:50	U	SMPL
PB129745BS - 1	LCSW	14566	3.8347	-7470A	PPB		25 Jun 2020 11:56:56	U	SMPL
L3087-02 - 1	FM1296	-67	0.0082	-7470A	PPB		25 Jun 2020 11:59:03	U	SMPL
L3087-02DUP - 1	FM1296DUP	-26	0.0189	-7470A	PPB		25 Jun 2020 12:01:09	U	SMPL
L3087-02MS - 1	FM1296MS	14290	3.7625	-7470A	PPB		25 Jun 2020 12:03:16	U	SMPL
L3087-02MSD - 1	FM1296MSD	15095	3.9730	-7470A	PPB		25 Jun 2020 12:05:23	U	SMPL
PB129746BL - 1	PBW	-58	0.0105	-7470A	PPB		25 Jun 2020 12:07:30	U	SMPL
PB129746BS - 1	LCSW	14275	3.7586	-7470A	PPB		25 Jun 2020 12:09:38	U	SMPL
L3087-01 - 1	FM1296	5706	1.5178	-7470A	PPB		25 Jun 2020 12:16:49	U	SMPL
L3087-01DUP - 1	FM1296DUP	5452	1.4514	-7470A	PPB		25 Jun 2020 12:18:55	U	SMPL
CCV78 - 1	CCV78	19757	5.1921	-7470A	PPB		25 Jun 2020 12:21:01	U	SMPL
CCB78 - 1	CCB78	-72	0.0069	-7470A	PPB		25 Jun 2020 12:23:07	U	SMPL
L3087-01MS - 1	FM1296MS	20682	5.4340	-7470A	PPB		25 Jun 2020 12:28:27	U	SMPL
L3087-01MSD - 1	FM1296MSD	20750	5.4518	-7470A	PPB		25 Jun 2020 12:30:33	U	SMPL
L3101-05 - 1	EBS8-W-04	-173	-0.0196	-7470A	PPB		25 Jun 2020 12:32:39	U	SMPL
PB129743TB - 1	PB129720TB	-88	0.0027	-7470A	PPB		25 Jun 2020 12:34:46	U	SMPL
PB129744TB - 1	PB129723TB	-8	0.0236	-7470A	PPB		25 Jun 2020 12:36:53	U	SMPL
PB129745TB - 1	PB129724TB	-7	0.0239	-7470A	PPB		25 Jun 2020 12:39:00	U	SMPL
L3094-03LX5 - 1		-11	0.0228	-7470A	PPB		25 Jun 2020 12:41:07	U	SMPL
L3094-03A - 1		14167	3.7303	-7470A	PPB		25 Jun 2020 12:43:14	U	SMPL
L3089-08LX5 - 1		-30	0.0178	-7470A	PPB		25 Jun 2020 12:45:22	U	SMPL
L3089-08A - 1		14439	3.8015	-7470A	PPB		25 Jun 2020 12:47:29	U	SMPL
CCV79 - 1	CCV79	19125	5.0269	-7470A	PPB		25 Jun 2020 12:49:35	U	SMPL
CCB79 - 1	CCB79	-55	0.0113	-7470A	PPB		25 Jun 2020 12:51:41	U	SMPL
L3087-02LX5 - 1		19	0.0307	-7470A	PPB		25 Jun 2020 12:53:47	U	SMPL
L3087-02A - 1		14585	3.8397	-7470A	PPB		25 Jun 2020 12:55:54	U	SMPL
L3087-01LX5 - 1		1043	0.2984	-7470A	PPB		25 Jun 2020 12:58:00	U	SMPL
L3087-01A - 1		20697	5.4379	-7470A	PPB		25 Jun 2020 13:00:06	U	SMPL
CCV80 - 1	CCV80	19560	5.1406	-7470A	PPB		25 Jun 2020 13:02:13	U	SMPL
CCB80 - 1	CCB80	-69	0.0076	-7470A	PPB		25 Jun 2020 13:04:20	U	SMPL