


LB109761

7471B

INSTRUMENT ID: CV1

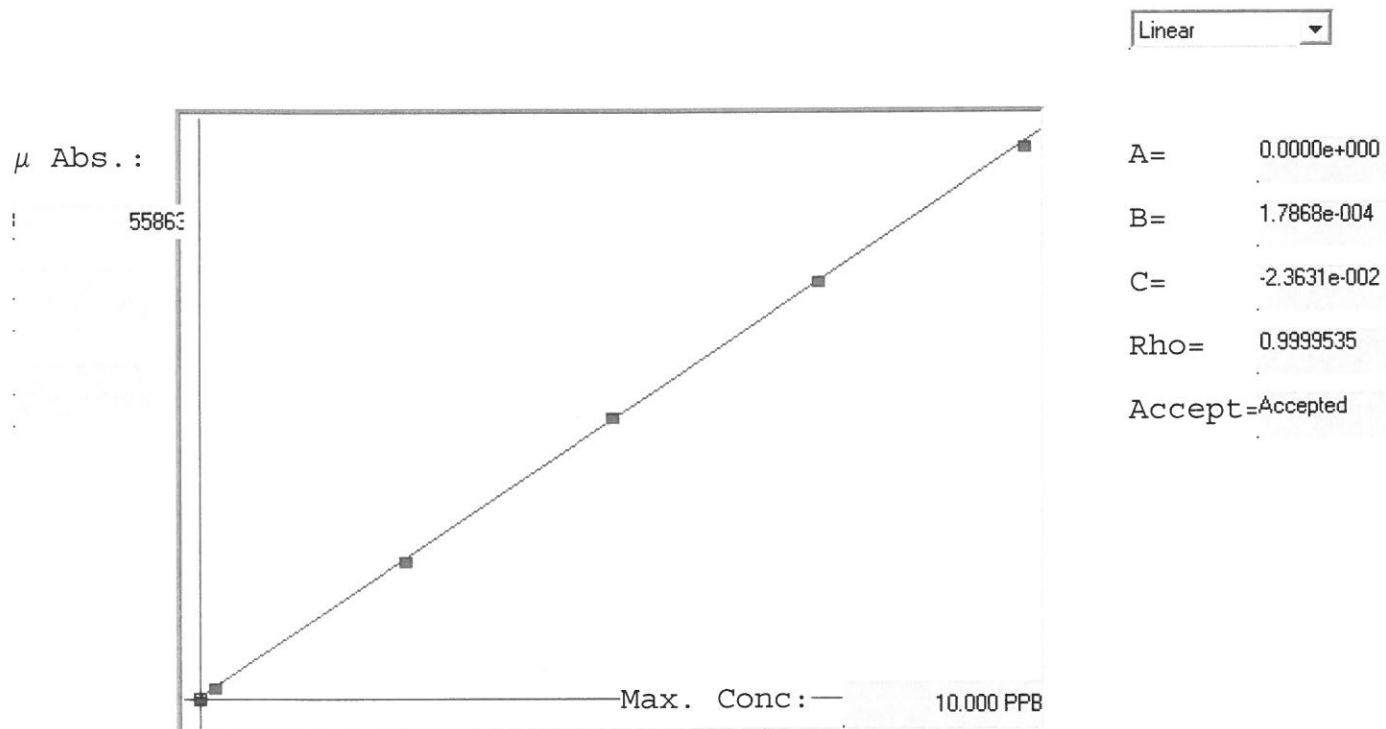

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.028	-0.028	-23	0.000	-23				
0.2	0.200	0.209	0.009	1301	0.0 %	1301				
2.5	2.500	2.477	-0.023	13997	0.0 %	13997				
5.0	5.000	5.064	0.064	28472	0.0 %	28472				
7.5	7.500	7.520	0.020	42220	0.0 %	42220				
10.0	10.000	9.958	-0.042	55863	0.0 %	55863				

LB109761 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 26 Jun 2020 13:43:04

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-23	-	0.0000	7471B	PPB	26 Jun 2020 13:45:01	S	Std
0.2 - 1	502	1301	-	0.2000	7471B	PPB	26 Jun 2020 13:47:17	S	Std
2.5 - 1	52.5	13997	-	2.5000	7471B	PPB	26 Jun 2020 13:49:34	S	Std
5.0 - 1	55	28472	-	5.0000	7471B	PPB	26 Jun 2020 13:51:51	S	Std
7.5 - 1	57.5	42220	-	7.5000	7471B	PPB	26 Jun 2020 13:54:07	S	Std
10.0 - 1	510	55863	-	10.0000	7471B	PPB	26 Jun 2020 14:00:55	S	Std
ICV02 - 1	ICV02	22622	4.0184	-	7471B	PPB	26 Jun 2020 14:03:35	U	SMPL
ICB02 - 1	ICB02	-139	-0.0485	-	7471B	PPB	26 Jun 2020 14:05:50	U	SMPL
CCV89 - 1	CCV89	28458	5.0612	-	7471B	PPB	26 Jun 2020 14:08:05	U	SMPL
CCB89 - 1	CCB89	-106	-0.0426	-	7471B	PPB	26 Jun 2020 14:10:20	U	SMPL
CRA - 1	CRA	1279	0.2049	-	7471B	PPB	26 Jun 2020 14:12:36	U	SMPL
HighStd - 1	HighStd	56808	10.1267	-	7471B	PPB	26 Jun 2020 14:14:51	U	SMPL
ChkStd - 1	ChkStd	40160	7.1520	-	7471B	PPB	26 Jun 2020 14:17:07	U	SMPL
PB129794BL - 1	PBS	-200	-0.0594	-	7471B	PPB	26 Jun 2020 14:19:24	U	SMPL
PB129794BS - 1	LCSS	21595	3.8349	-	7471B	PPB	26 Jun 2020 14:21:42	U	SMPL
L3113-01 - 1	DRUM-COMP	9704	1.7103	-	7471B	PPB	26 Jun 2020 14:23:58	U	SMPL
L3113-01DUP - 1	DRUM-COMPDUP	8088	1.4215	-	7471B	PPB	26 Jun 2020 14:26:15	U	SMPL
L3113-01MS - 1	DRUM-COMPMS	31774	5.6537	-	7471B	PPB	26 Jun 2020 14:28:33	U	SMPL
L3113-01MSD - 1	DRUM-COMPMSD	31727	5.6453	-	7471B	PPB	26 Jun 2020 14:30:50	U	SMPL
L3114-01 - 1	VNJ-242	1339	0.2156	-	7471B	PPB	26 Jun 2020 14:33:06	U	SMPL
CCV90 - 1	CCV90	28748	5.1130	-	7471B	PPB	26 Jun 2020 14:35:23	U	SMPL
CCB90 - 1	CCB90	-113	-0.0438	-	7471B	PPB	26 Jun 2020 14:37:38	U	SMPL
L3115-01 - 1	TP	1604	0.2630	-	7471B	PPB	26 Jun 2020 14:39:54	U	SMPL
L3126-03 - 1	TP-8-S	1880	0.3123	-	7471B	PPB	26 Jun 2020 14:42:10	U	SMPL
L3126-07 - 1	TP-7-S	6353	1.1115	-	7471B	PPB	26 Jun 2020 14:44:25	U	SMPL
L3126-11 - 1	TP-4-S	21551	3.8270	-	7471B	PPB	26 Jun 2020 14:46:41	U	SMPL
L3113-01LX5 - 1		1728	0.2851	-	7471B	PPB	26 Jun 2020 14:48:57	U	SMPL
L3113-01A - 1		31766	5.6522	-	7471B	PPB	26 Jun 2020 14:51:13	U	SMPL
CCV91 - 1	CCV91	28856	5.1323	-	7471B	PPB	26 Jun 2020 14:53:29	U	SMPL
CCB91 - 1	CCB91	-131	-0.0470	-	7471B	PPB	26 Jun 2020 14:55:47	U	SMPL