


LB169819

245.1

INSTRUMENT ID: CV1

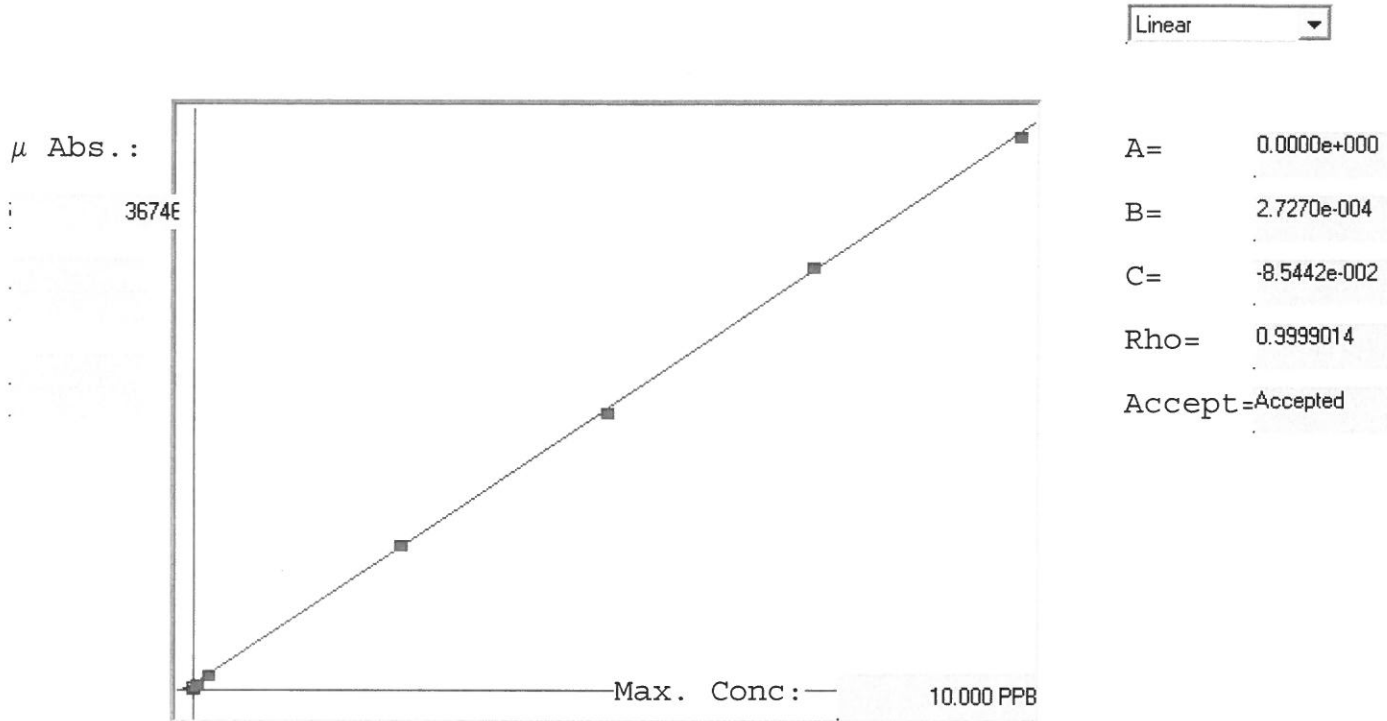

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.048	-0.048	139	0.000	139				
0.05	0.050	0.041	-0.009	464	0.0 %	464				
0.2	0.200	0.196	-0.004	1033	0.0 %	1033				
2.5	2.500	2.575	0.075	9757	0.0 %	9757				
5.0	5.000	4.972	-0.028	18547	0.0 %	18547				
7.5	7.500	7.578	0.078	28101	0.0 %	28101				
10.0	10.000	9.935	-0.065	36746	0.0 %	36746				

LB109819 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 01 Jul 2020 12:34:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	139	-	0.0000	245.1	PPB	01 Jul 2020 12:35:52	S	Std
0.05 - 1	50.05	464	-	0.0500	245.1	PPB	01 Jul 2020 12:38:08	S	Std
0.2 - 1	50.2	1033	-	0.2000	245.1	PPB	01 Jul 2020 12:40:25	S	Std
2.5 - 1	52.5	9757	-	2.5000	245.1	PPB	01 Jul 2020 12:42:42	S	Std
5.0 - 1	55	18547	-	5.0000	245.1	PPB	01 Jul 2020 12:44:59	S	Std
7.5 - 1	57.5	28101	-	7.5000	245.1	PPB	01 Jul 2020 12:47:15	S	Std
10.0 - 1	510	36746	-	10.0000	245.1	PPB	01 Jul 2020 13:00:46	S	Std
ICV09 - 1	ICV09	15217	4.0642	-245.1		PPB	01 Jul 2020 13:03:30	U	SMPL
ICB09 - 1	ICB09	20	-0.0800	-245.1		PPB	01 Jul 2020 13:05:44	U	SMPL
CCV20 - 1	CCV20	18373	4.9248	-245.1		PPB	01 Jul 2020 13:08:00	U	SMPL
CCB20 - 1	CCB20	16	-0.0811	-245.1		PPB	01 Jul 2020 13:10:15	U	SMPL
CRA - 1	CRA	450	0.0373	-245.1		PPB	01 Jul 2020 13:17:59	U	SMPL
HighStd - 1	HighStd	36370	9.8325	-245.1		PPB	01 Jul 2020 13:20:13	U	SMPL
ChkStd - 1	ChkStd	26417	7.1184	-245.1		PPB	01 Jul 2020 13:22:29	U	SMPL
PB129901BL - 1	PBW	192	-0.0331	-245.1		PPB	01 Jul 2020 13:24:46	U	SMPL
PB129901BS - 1	LCSW	14564	3.8861	-245.1		PPB	01 Jul 2020 13:27:02	U	SMPL
L3155-01 - 1	MH-D19	2643	0.6353	-245.1		PPB	01 Jul 2020 13:29:19	U	SMPL
L3155-01DUP - 1	MH-D19DUP	2746	0.6634	-245.1		PPB	01 Jul 2020 13:34:15	U	SMPL
L3155-01MS - 1	MH-D19MS	16219	4.3374	-245.1		PPB	01 Jul 2020 13:36:32	U	SMPL
L3155-01MSD - 1	MH-D19MSD	16106	4.3066	-245.1		PPB	01 Jul 2020 13:38:49	U	SMPL
L3155-04 - 1	MH-D19	5	-0.0841	-245.1		PPB	01 Jul 2020 13:41:05	U	SMPL
CCV21 - 1	CCV21	18245	4.8899	-245.1		PPB	01 Jul 2020 13:43:20	U	SMPL
CCB21 - 1	CCB21	32	-0.0767	-245.1		PPB	01 Jul 2020 13:45:35	U	SMPL
L3155-01LX5 - 1		585	0.0741	-245.1		PPB	01 Jul 2020 13:47:51	U	SMPL
L3155-01A - 1		16105	4.3063	-245.1		PPB	01 Jul 2020 13:50:06	U	SMPL
CCV22 - 1	CCV22	17707	4.7432	-245.1		PPB	01 Jul 2020 13:52:22	U	SMPL
CCB22 - 1	CCB22	15	-0.0814	-245.1		PPB	01 Jul 2020 13:54:38	U	SMPL