


LB109841

7470A

INSTRUMENT ID: CV1

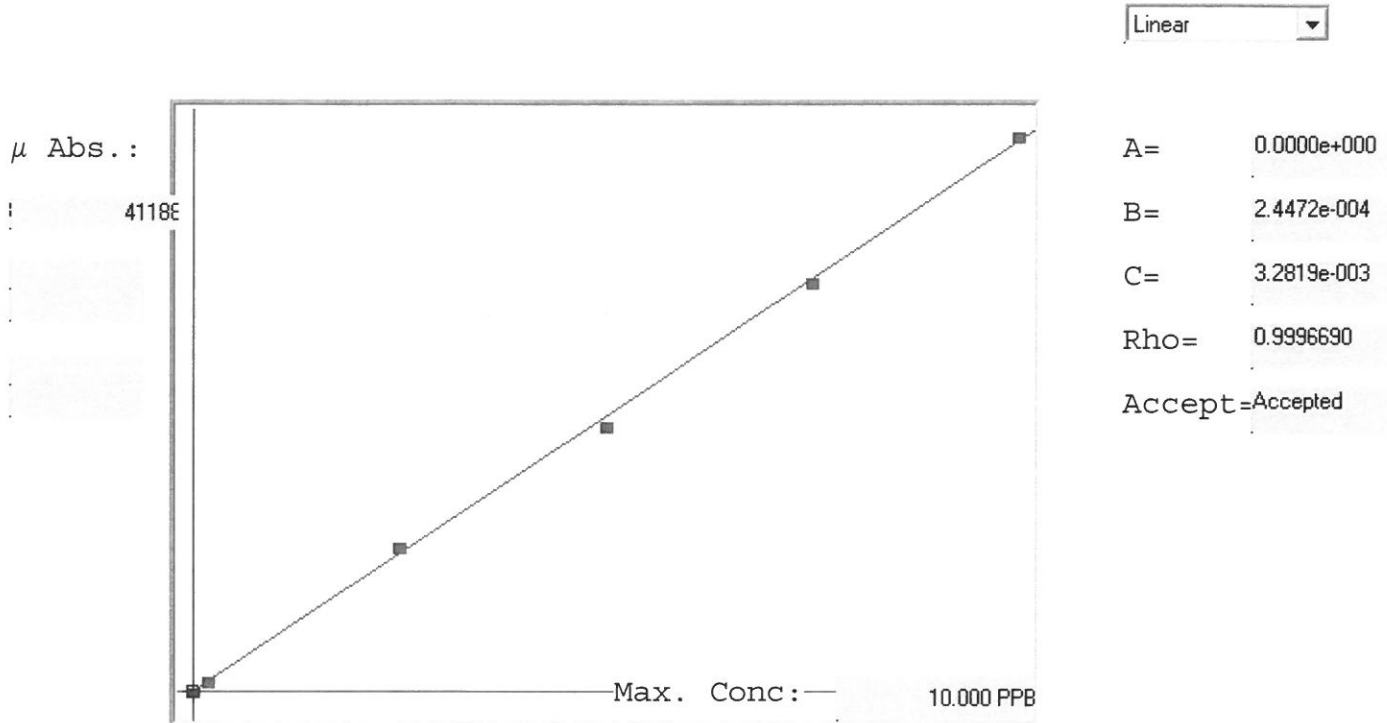

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.008	0.008	20	0.000	20				
0.2	0.200	0.191	-0.009	768	0.0 %	768				
2.5	2.500	2.634	0.134	10749	0.0 %	10749				
5.0	5.000	4.838	-0.162	19756	0.0 %	19756				
7.5	7.500	7.446	-0.054	30413	0.0 %	30413				
10.0	10.000	10.083	0.083	41188	0.0 %	41188				

LB109841 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 02 Jul 2020 12:16:27

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	20	-	0.0000	7470A	PPB	02 Jul 2020 12:59:23	S	Std
0.2 - 1	50.2	768	-	0.2000	7470A	PPB	02 Jul 2020 13:01:31	S	Std
2.5 - 1	52.5	10749	-	2.5000	7470A	PPB	02 Jul 2020 13:03:39	S	Std
5.0 - 1	55	19756	-	5.0000	7470A	PPB	02 Jul 2020 13:05:47	S	Std
7.5 - 1	57.5	30413	-	7.5000	7470A	PPB	02 Jul 2020 13:07:53	S	Std
10.0 - 1	510	41188	-	10.0000	7470A	PPB	02 Jul 2020 13:10:00	S	Std
ICV12 - 1	ICV12	16672	4.0833	-7470A	PPB	02 Jul 2020 13:20:00	U	SMPL	
ICB12 - 1	ICB12	-82	-0.0168	-7470A	PPB	02 Jul 2020 13:22:06	U	SMPL	
CCV30 - 1	CCV30	20073	4.9156	-7470A	PPB	02 Jul 2020 13:24:12	U	SMPL	
CCB30 - 1	CCB30	-63	-0.0121	-7470A	PPB	02 Jul 2020 13:26:17	U	SMPL	
CRA - 1	CRA	778	0.1937	-7470A	PPB	02 Jul 2020 13:28:23	U	SMPL	
HighStd - 1	HighStd	41447	10.1462	-7470A	PPB	02 Jul 2020 13:30:28	U	SMPL	
ChkStd - 1	ChkStd	27162	6.6504	-7470A	PPB	02 Jul 2020 13:32:34	U	SMPL	
PB129941BL - 1	PBW	-80	-0.0163	-7470A	PPB	02 Jul 2020 13:34:42	U	SMPL	
PB129941BS - 1	LCSW	15910	3.8968	-7470A	PPB	02 Jul 2020 13:36:50	U	SMPL	
L3173-01 - 1	13854	40	0.0131	-7470A	PPB	02 Jul 2020 13:38:57	U	SMPL	
L3188-04 - 1	TR-04-070120	-8	0.0013	-7470A	PPB	02 Jul 2020 13:41:04	U	SMPL	
L3197-03 - 1	MH-1-COMP	0	0.0033	-7470A	PPB	02 Jul 2020 13:43:12	U	SMPL	
L3197-09 - 1	MH-2-COMP	20	0.0082	-7470A	PPB	02 Jul 2020 13:45:19	U	SMPL	
L3197-09DUP - 1	MH-2-COMPDUP	19	0.0079	-7470A	PPB	02 Jul 2020 13:47:25	U	SMPL	
CCV31 - 1	CCV31	19623	4.8054	-7470A	PPB	02 Jul 2020 13:52:03	U	SMPL	
CCB31 - 1	CCB31	-53	-0.0097	-7470A	PPB	02 Jul 2020 13:54:09	U	SMPL	
L3197-09MS - 1	MH-2-COMPMS	15822	3.8753	-7470A	PPB	02 Jul 2020 13:56:14	U	SMPL	
L3197-09MSD - 1	MH-2-COMPMSD	15831	3.8775	-7470A	PPB	02 Jul 2020 13:58:20	U	SMPL	
PB129942BL - 1	PBW	-59	-0.0112	-7470A	PPB	02 Jul 2020 14:00:27	U	SMPL	
PB129942BS - 1	LCSW	14792	3.6232	-7470A	PPB	02 Jul 2020 14:02:33	U	SMPL	
L3195-07 - 1	RB-01-20200630	-105	-0.0224	-7470A	PPB	02 Jul 2020 14:04:39	U	SMPL	
L3198-01 - 1	MW-2R	-21	-0.0019	-7470A	PPB	02 Jul 2020 14:06:47	U	SMPL	
L3198-02 - 1	MW-12	12	0.0062	-7470A	PPB	02 Jul 2020 14:08:54	U	SMPL	
L3198-03 - 1	MW-1	26	0.0096	-7470A	PPB	02 Jul 2020 14:11:02	U	SMPL	
L3198-04 - 1	MW-10	-47	-0.0082	-7470A	PPB	02 Jul 2020 14:13:11	U	SMPL	
L3198-05 - 1	SW-1	-64	-0.0124	-7470A	PPB	02 Jul 2020 14:15:17	U	SMPL	
CCV32 - 1	CCV32	20193	4.9449	-7470A	PPB	02 Jul 2020 14:17:23	U	SMPL	
CCB32 - 1	CCB32	-52	-0.0094	-7470A	PPB	02 Jul 2020 14:19:29	U	SMPL	
L3198-05DUP - 1	SW-1DUP	-35	-0.0053	-7470A	PPB	02 Jul 2020 14:21:36	U	SMPL	
L3198-06 - 1	L3198-05MS	13768	3.3726	-7470A	PPB	02 Jul 2020 14:23:42	U	SMPL	
L3198-07 - 1	L3198-05MSD	14179	3.4732	-7470A	PPB	02 Jul 2020 14:25:48	U	SMPL	
L3198-08 - 1	MW-6R	25	0.0094	-7470A	PPB	02 Jul 2020 14:27:55	U	SMPL	
PB129941TB - 1	PB129916TB	-16	-0.0006	-7470A	PPB	02 Jul 2020 14:30:01	U	SMPL	
L3197-09LX5 - 1		9	0.0055	-7470A	PPB	02 Jul 2020 14:32:08	U	SMPL	
L3197-09A - 1		16094	3.9418	-7470A	PPB	02 Jul 2020 14:34:15	U	SMPL	
L3198-05LX5 - 1		-70	-0.0138	-7470A	PPB	02 Jul 2020 14:36:23	U	SMPL	
L3198-05A - 1		17014	4.1670	-7470A	PPB	02 Jul 2020 14:38:31	U	SMPL	
CCV33 - 1	CCV33	19944	4.8840	-7470A	PPB	02 Jul 2020 14:40:38	U	SMPL	
CCB33 - 1	CCB33	-61	-0.0116	-7470A	PPB	02 Jul 2020 14:42:44	U	SMPL	