


LB109887

7471B

INSTRUMENT ID: CV1

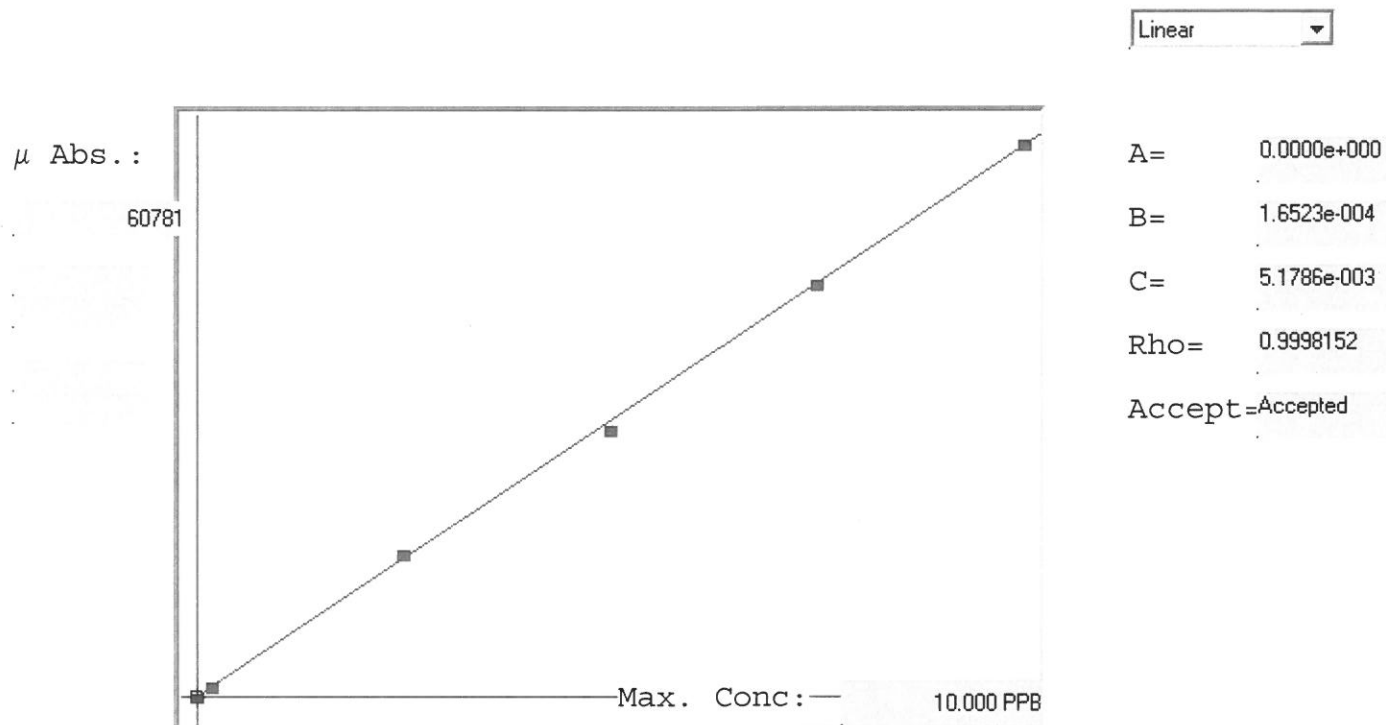

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.003	0.003	-13	0.000	-13				
0.2	0.200	0.211	0.011	1245	0.0 %	1245				
2.5	2.500	2.582	0.082	15596	0.0 %	15596				
5.0	5.000	4.855	-0.145	29352	0.0 %	29352				
7.5	7.500	7.501	0.001	45368	0.0 %	45368				
10.0	10.000	10.048	0.048	60781	0.0 %	60781				

LB109887 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 07 Jul 2020 12:09:48

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	-13	-	0.00007471B	PPB	07 Jul 2020 12:11:18	S	Std
0.2 - 1	50.2	1245	-	0.20007471B	PPB	07 Jul 2020 12:13:35	S	Std
2.5 - 1	52.5	15596	-	2.50007471B	PPB	07 Jul 2020 12:15:52	S	Std
5.0 - 1	55	29352	-	5.00007471B	PPB	07 Jul 2020 12:18:09	S	Std
7.5 - 1	57.5	45368	-	7.50007471B	PPB	07 Jul 2020 12:20:25	S	Std
10.0 - 1	58	60781	-	10.00007471B	PPB	07 Jul 2020 12:22:42	S	Std
ICV16 - 1	ICV16	24470	4.0483	-7471B	PPB	07 Jul 2020 12:25:27	U	SMPL
ICB16 - 1	ICB16	-129	-0.0161	-7471B	PPB	07 Jul 2020 12:27:41	U	SMPL
CCV51 - 1	CCV51	28970	4.7918	-7471B	PPB	07 Jul 2020 12:29:57	U	SMPL
CCB51 - 1	CCB51	-146	-0.0189	-7471B	PPB	07 Jul 2020 12:32:12	U	SMPL
CRA - 1	CRA	1204	0.2041	-7471B	PPB	07 Jul 2020 12:34:27	U	SMPL
HighStd - 1	HighStd	61192	10.1158	-7471B	PPB	07 Jul 2020 12:36:43	U	SMPL
ChkStd - 1	ChkStd	40808	6.7478	-7471B	PPB	07 Jul 2020 12:38:58	U	SMPL
PB130001BL - 1	PBS	-211	-0.0297	-7471B	PPB	07 Jul 2020 12:41:15	U	SMPL
PB130001BS - 1	LCSS	24642	4.0767	-7471B	PPB	07 Jul 2020 12:43:32	U	SMPL
L3217-01 - 1	E3-41-DRUM-95	-35	-0.0006	-7471B	PPB	07 Jul 2020 12:45:49	U	SMPL
L3217-02 - 1	E3-41-NHS	630379	HIGH	-7471B	PPB	07 Jul 2020 12:48:05	X	
L3217-03 - 1	E3-41-COMP-1-FLOOR	36192	5.9851	-7471B	PPB	07 Jul 2020 12:49:55	U	SMPL
L3217-04 - 1	E3-41-VAT	25754	4.2604	-7471B	PPB	07 Jul 2020 12:52:25	U	SMPL
L3217-05 - 1	E3-41-BOILER-ROOM	50841	8.4055	-7471B	PPB	07 Jul 2020 12:54:42	U	SMPL
CCV52 - 1	CCV52	28700	4.7472	-7471B	PPB	07 Jul 2020 12:56:58	U	SMPL
CCB52 - 1	CCB52	-161	-0.0214	-7471B	PPB	07 Jul 2020 12:59:16	U	SMPL
L3228-01 - 1	VNJ-217	3163	0.5278	-7471B	PPB	07 Jul 2020 13:01:32	U	SMPL
L3230-01 - 1	FK-BPM-01-C4-D4-C4A-D4A	1644	0.2768	-7471B	PPB	07 Jul 2020 13:03:48	U	SMPL
L3230-01DUP - 1	FK-BPM-01-C4-D4-C4A-D4ADUP	1598	0.2692	-7471B	PPB	07 Jul 2020 13:06:04	U	SMPL
L3230-01MS - 1	FK-BPM-01-C4-D4-C4A-D4AMS	24533	4.0587	-7471B	PPB	07 Jul 2020 13:08:19	U	SMPL
L3230-01MSD - 1	FK-BPM-01-C4-D4-C4A-D4AMSD	24318	4.0232	-7471B	PPB	07 Jul 2020 13:10:35	U	SMPL
L3217-02DLX10 - 1		131080	21.6632	-7471B	PPB	07 Jul 2020 13:12:52	U	SMPL
L3230-01LX5 - 1		279	0.0513	-7471B	PPB	07 Jul 2020 13:19:09	U	SMPL
L3230-01A - 1		25032	4.1412	-7471B	PPB	07 Jul 2020 13:21:25	U	SMPL
L3217-02DLX50 - 1		26893	4.4486	-7471B	PPB	07 Jul 2020 13:23:42	U	SMPL
CCV53 - 1	CCV53	28689	4.7454	-7471B	PPB	07 Jul 2020 13:25:57	U	SMPL
CCB53 - 1	CCB53	-133	-0.0168	-7471B	PPB	07 Jul 2020 13:28:14	U	SMPL