


LB109910

7471B INSTRUMENT ID: CV1

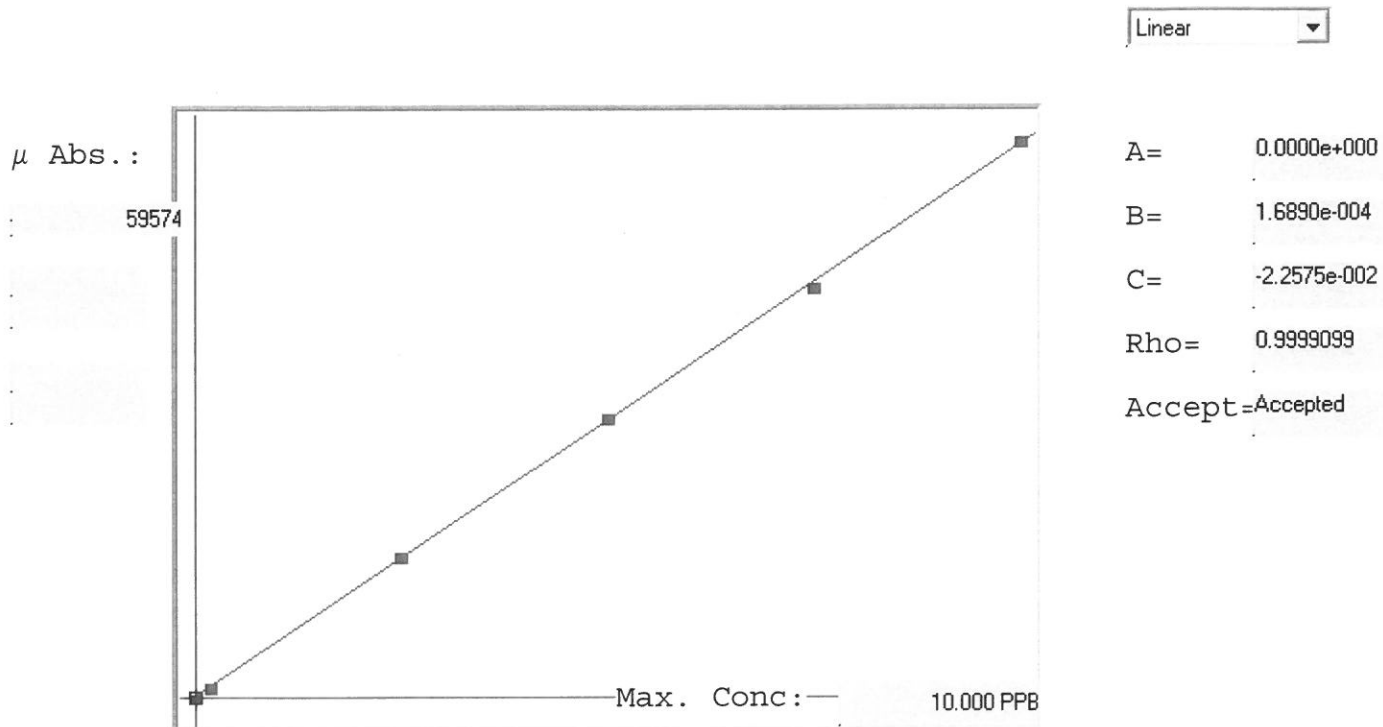

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.010	-0.010	74	0.000	74				
0.2	0.200	0.186	-0.014	1235	0.0 %	1235				
2.5	2.500	2.534	0.034	15139	0.0 %	15139				
5.0	5.000	5.048	0.048	30019	0.0 %	30019				
7.5	7.500	7.403	-0.097	43964	0.0 %	43964				
10.0	10.000	10.039	0.039	59574	0.0 %	59574				

LB109910 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Jul 2020 11:47:52

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	74	-	0.00007471B	PPB	08 Jul 2020 11:51:44	S	Std
0.2 - 1	50.2	1235	-	0.20007471B	PPB	08 Jul 2020 11:54:00	S	Std
2.5 - 1	52.5	15139	-	2.50007471B	PPB	08 Jul 2020 11:56:17	S	Std
5.0 - 1	55	30019	-	5.00007471B	PPB	08 Jul 2020 11:58:34	S	Std
7.5 - 1	57.5	43964	-	7.50007471B	PPB	08 Jul 2020 12:00:50	S	Std
10.0 - 1	510	59574	-	10.00007471B	PPB	08 Jul 2020 12:05:45	S	Std
ICV18 - 1	ICV18	24556	4.1249	-7471B	PPB	08 Jul 2020 12:10:52	U	SMPL
ICB18 - 1	ICB18	22	-0.0189	-7471B	PPB	08 Jul 2020 12:13:07	U	SMPL
CCV57 - 1	CCV57	29177	4.9053	-7471B	PPB	08 Jul 2020 12:15:23	U	SMPL
CCB57 - 1	CCB57	10	-0.0209	-7471B	PPB	08 Jul 2020 12:17:38	U	SMPL
CRA - 1	CRA	1193	0.1789	-7471B	PPB	08 Jul 2020 12:19:55	U	SMPL
HighStd - 1	HighStd	59262	9.9866	-7471B	PPB	08 Jul 2020 12:22:10	U	SMPL
ChkStd - 1	ChkStd	42875	7.2189	-7471B	PPB	08 Jul 2020 12:24:26	U	SMPL
PB130026BL - 1	PBS	-83	-0.0366	-7471B	PPB	08 Jul 2020 12:26:43	U	SMPL
PB130026BS - 1	LCSS	20616	3.4594	-7471B	PPB	08 Jul 2020 12:28:59	U	SMPL
L3183-01 - 1	OK-02-070720	818	0.1156	-7471B	PPB	08 Jul 2020 12:31:16	U	SMPL
L3187-01 - 1	SU-02-070720	1885	0.2958	-7471B	PPB	08 Jul 2020 12:33:32	U	SMPL
L3187-01DUP - 1	SU-02-070720DUP	1944	0.3058	-7471B	PPB	08 Jul 2020 12:35:49	U	SMPL
L3187-01MS - 1	SU-02-070720MS	23957	4.0237	-7471B	PPB	08 Jul 2020 12:38:06	U	SMPL
L3187-01MSD - 1	SU-02-070720MSD	23643	3.9707	-7471B	PPB	08 Jul 2020 12:40:21	U	SMPL
CCV58 - 1	CCV58	29182	4.9062	-7471B	PPB	08 Jul 2020 12:42:37	U	SMPL
CCB58 - 1	CCB58	6	-0.0216	-7471B	PPB	08 Jul 2020 12:44:52	U	SMPL
L3203-01 - 1	RO-24	1572	0.2429	-7471B	PPB	08 Jul 2020 12:47:08	U	SMPL
L3203-05 - 1	RO-10	10994	1.8343	-7471B	PPB	08 Jul 2020 12:49:23	U	SMPL
L3203-09 - 1	RO-20	12970	2.1680	-7471B	PPB	08 Jul 2020 12:51:39	U	SMPL
L3203-13 - 1	RO-06	2398	0.3824	-7471B	PPB	08 Jul 2020 12:53:55	U	SMPL
L3203-17 - 1	RO-16	3782	0.6162	-7471B	PPB	08 Jul 2020 12:56:11	U	SMPL
L3187-01LX5 - 1		370	0.0399	-7471B	PPB	08 Jul 2020 12:58:27	U	SMPL
L3187-01A - 1		24429	4.1034	-7471B	PPB	08 Jul 2020 13:00:44	U	SMPL
CCV59 - 1	CCV59	29063	4.8861	-7471B	PPB	08 Jul 2020 13:03:00	U	SMPL
CCB59 - 1	CCB59	15	-0.0200	-7471B	PPB	08 Jul 2020 13:05:17	U	SMPL