


L3109921

7470A

INSTRUMENT ID: CY1

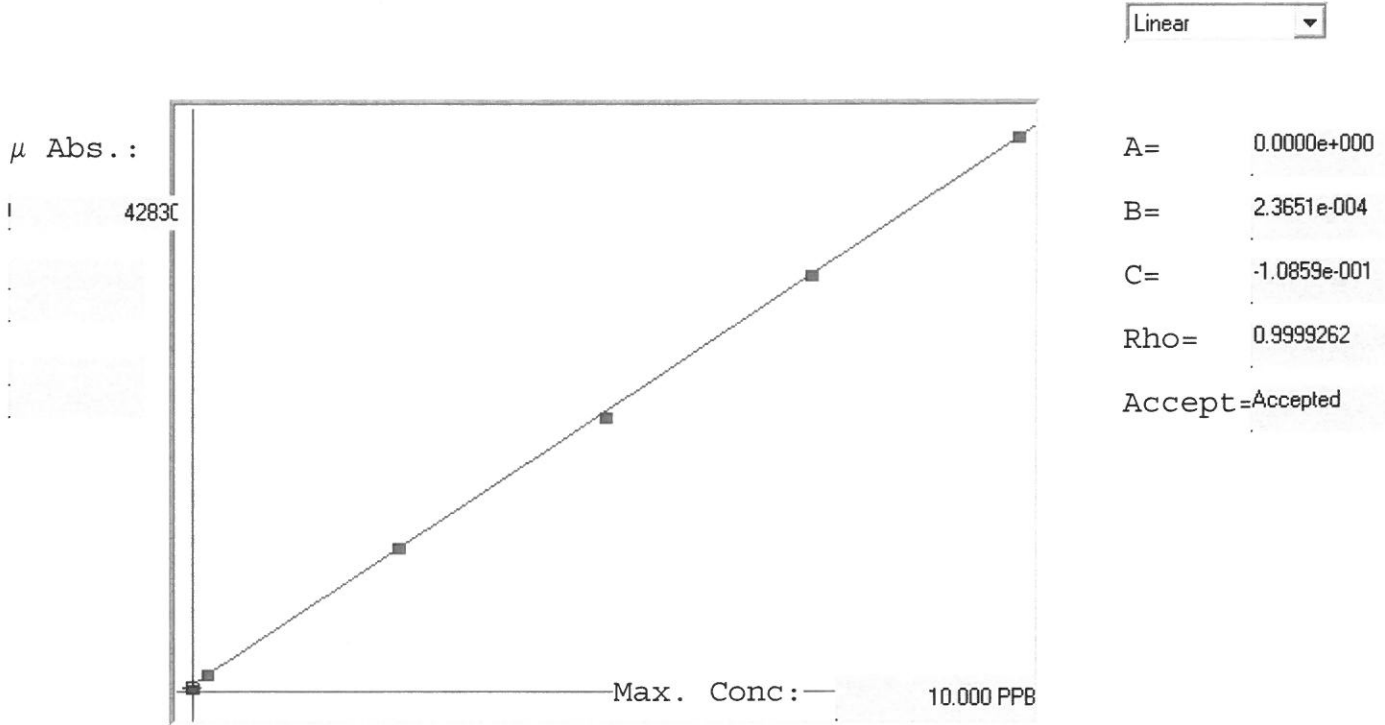

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.019	-0.019	378	0.000	378				
0.2	0.200	0.234	0.034	1448	0.0 %	1448				
2.5	2.500	2.538	0.038	11190	0.0 %	11190				
5.0	5.000	4.909	-0.091	21214	0.0 %	21214				
7.5	7.500	7.518	0.018	32246	0.0 %	32246				
10.0	10.000	10.021	0.021	42830	0.0 %	42830				

LB109921 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 09 Jul 2020 11:30:47					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	378	-	0.0000	7470A	PPB	09 Jul 2020 11:34:21	S	Std
0.2 - 1	50.2	1448	-	0.2000	7470A	PPB	09 Jul 2020 11:36:28	S	Std
2.5 - 1	52.5	11190	-	2.5000	7470A	PPB	09 Jul 2020 11:38:36	S	Std
5.0 - 1	55	21214	-	5.0000	7470A	PPB	09 Jul 2020 11:40:44	S	Std
7.5 - 1	57.5	32246	-	7.5000	7470A	PPB	09 Jul 2020 11:42:51	S	Std
10.0 - 1	510	42830	-	10.0000	7470A	PPB	09 Jul 2020 11:49:47	S	Std
ICV20 - 1	ICV20	16789	3.8621	-	7470A	PPB	09 Jul 2020 11:52:18	U	SMPL
ICB20 - 1	ICB20	342	-0.0277	-	7470A	PPB	09 Jul 2020 11:54:23	U	SMPL
CCV66 - 1	CCV66	21399	4.9524	-	7470A	PPB	09 Jul 2020 11:56:30	U	SMPL
CCB66 - 1	CCB66	331	-0.0303	-	7470A	PPB	09 Jul 2020 11:58:35	U	SMPL
CRA - 1	CRA	1510	0.2485	-	7470A	PPB	09 Jul 2020 12:00:41	U	SMPL
HighStd - 1	HighStd	42580	9.9618	-	7470A	PPB	09 Jul 2020 12:02:47	U	SMPL
ChkStd - 1	ChkStd	28808	6.7047	-	7470A	PPB	09 Jul 2020 12:04:53	U	SMPL
PB130056BL - 1	PBW	427	-0.0076	-	7470A	PPB	09 Jul 2020 12:18:17	U	SMPL
PB130056BS - 1	LCSW	15681	3.6001	-	7470A	PPB	09 Jul 2020 12:25:12	U	SMPL
L3217-07 - 1	E3-41-ACID	6845	1.5103	-	7470A	PPB	09 Jul 2020 12:27:19	U	SMPL
CCV67 - 1	CCV67	20483	4.7358	-	7470A	PPB	09 Jul 2020 12:29:26	U	SMPL
CCB67 - 1	CCB67	240	-0.0518	-	7470A	PPB	09 Jul 2020 12:31:34	U	SMPL