


LB 109943

7470A

INSTRUMENT ID: CY1

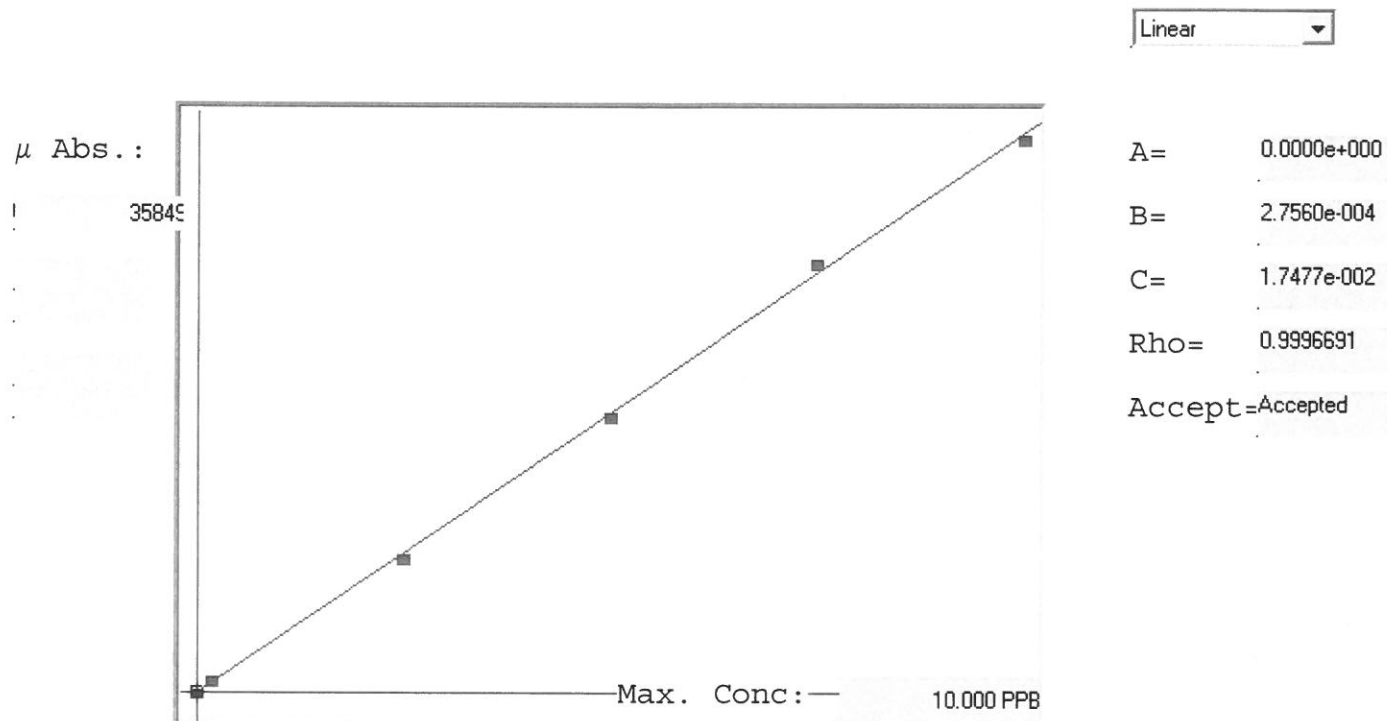

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.021	0.021	11	0.000	11				
0.2	0.200	0.223	0.023	747	0.0 %	747				
2.5	2.500	2.414	-0.086	8696	0.0 %	8696				
5.0	5.000	4.961	-0.039	17938	0.0 %	17938				
7.5	7.500	7.684	0.184	27816	0.0 %	27816				
10.0	10.000	9.897	-0.103	35849	0.0 %	35849				

LB109943 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 10 Jul 2020 10:01:55

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	11	-	0.00007470A		PPB	10 Jul 2020 10:05:16	S	Std
0.2 - 1	52.2	747	-	0.20007470A		PPB	10 Jul 2020 10:07:24	S	Std
2.5 - 1	52.5	8696	-	2.50007470A		PPB	10 Jul 2020 10:09:32	S	Std
5.0 - 1	55	17938	-	5.00007470A		PPB	10 Jul 2020 10:11:40	S	Std
7.5 - 1	57.5	27816	-	7.50007470A		PPB	10 Jul 2020 10:13:47	S	Std
10.0 - 1	510	35849	-	10.00007470A		PPB	10 Jul 2020 10:15:54	S	Std
ICV22 - 1	ICV22	14036	3.8858	-7470A		PPB	10 Jul 2020 10:18:40	U	SMPL
ICB22 - 1	ICB22	-130	-0.0184	-7470A		PPB	10 Jul 2020 10:20:46	U	SMPL
CCV71 - 1	CCV71	17701	4.8958	-7470A		PPB	10 Jul 2020 10:22:51	U	SMPL
CCB71 - 1	CCB71	-149	-0.0236	-7470A		PPB	10 Jul 2020 10:24:57	U	SMPL
CRA - 1	CRA	726	0.2176	-7470A		PPB	10 Jul 2020 10:27:03	U	SMPL
HighStd - 1	HighStd	36626	10.1115	-7470A		PPB	10 Jul 2020 10:29:09	U	SMPL
ChkStd - 1	ChkStd	25683	7.0957	-7470A		PPB	10 Jul 2020 10:31:15	U	SMPL
PB130082BL - 1	PBW	-252	-0.0520	-7470A		PPB	10 Jul 2020 10:33:22	U	SMPL
PB130082BS - 1	LCSW	12998	3.5997	-7470A		PPB	10 Jul 2020 10:35:31	U	SMPL
L3186-05 - 1	OR-02-070820	-140	-0.0211	-7470A		PPB	10 Jul 2020 10:37:38	U	SMPL
L3186-05DUP - 1	OR-02-070820DUP	-62	0.0004	-7470A		PPB	10 Jul 2020 10:39:45	U	SMPL
L3186-05MS - 1	OR-02-070820MS	12208	3.3820	-7470A		PPB	10 Jul 2020 10:41:53	U	SMPL
L3186-05MSD - 1	OR-02-070820MSD	13168	3.6466	-7470A		PPB	10 Jul 2020 10:44:01	U	SMPL
L3203-03 - 1	RO-24	-160	-0.0266	-7470A		PPB	10 Jul 2020 10:46:07	U	SMPL
CCV72 - 1	CCV72	18105	5.0072	-7470A		PPB	10 Jul 2020 10:48:13	U	SMPL
CCB72 - 1	CCB72	-182	-0.0327	-7470A		PPB	10 Jul 2020 10:50:19	U	SMPL
L3203-07 - 1	RO-10	-63	0.0001	-7470A		PPB	10 Jul 2020 10:52:26	U	SMPL
L3203-11 - 1	RO-20	-26	0.0103	-7470A		PPB	10 Jul 2020 10:54:32	U	SMPL
L3203-15 - 1	RO-06	-41	0.0062	-7470A		PPB	10 Jul 2020 10:56:38	U	SMPL
L3203-19 - 1	RO-16	-28	0.0098	-7470A		PPB	10 Jul 2020 10:58:45	U	SMPL
PB130083BL - 1	PBW	-31	0.0089	-7470A		PPB	10 Jul 2020 11:00:52	U	SMPL
PB130083BS - 1	LCSW	12538	3.4729	-7470A		PPB	10 Jul 2020 11:02:59	U	SMPL
L3250-10 - 1	DRUM-VAULT-WATER-COMP-2	-120	-0.0156	-7470A		PPB	10 Jul 2020 11:05:06	U	SMPL
L3250-10DUP - 1	DRUM-VAULT-WATER-COMP-2DUP	-38	0.0070	-7470A		PPB	10 Jul 2020 11:07:14	U	SMPL
L3250-10MS - 1	DRUM-VAULT-WATER-COMP-2MS	13867	3.8392	-7470A		PPB	10 Jul 2020 11:09:21	U	SMPL
L3250-10MSD - 1	DRUM-VAULT-WATER-COMP-2MSD	13335	3.6926	-7470A		PPB	10 Jul 2020 11:11:28	U	SMPL
CCV73 - 1	CCV73	18472	5.1083	-7470A		PPB	10 Jul 2020 11:13:34	U	SMPL
CCB73 - 1	CCB73	-207	-0.0396	-7470A		PPB	10 Jul 2020 11:15:41	U	SMPL
PB130082TB - 1	PB130034TB	-68	-0.0013	-7470A		PPB	10 Jul 2020 11:17:47	U	SMPL
PB130083TB - 1	PB130075TB	-46	0.0048	-7470A		PPB	10 Jul 2020 11:19:53	U	SMPL
L3186-05LX5 - 1		-28	0.0098	-7470A		PPB	10 Jul 2020 11:22:00	U	SMPL
L3186-05A - 1		14135	3.9131	-7470A		PPB	10 Jul 2020 11:24:06	U	SMPL
L3250-10LX5 - 1		-132	-0.0189	-7470A		PPB	10 Jul 2020 11:26:13	U	SMPL
L3250-10A - 1		14318	3.9635	-7470A		PPB	10 Jul 2020 11:28:20	U	SMPL
CCV74 - 1	CCV74	18140	5.0168	-7470A		PPB	10 Jul 2020 11:30:28	U	SMPL
CCB74 - 1	CCB74	-216	-0.0421	-7470A		PPB	10 Jul 2020 11:32:36	U	SMPL