


LB109953

ISM02.4

INSTRUMENT ID: CVI

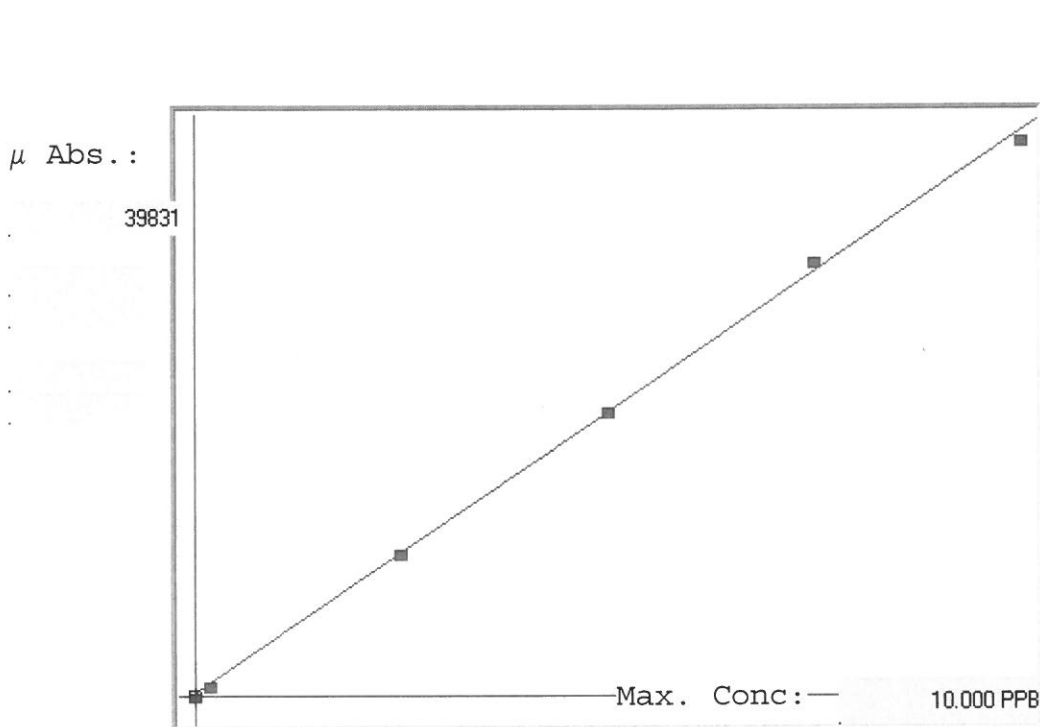

A= 0.0000e+000

B= 2.4759e-004

C= -3.8281e-002

Rho= 0.9995317

Accept=Accepted

slope
 $4.1271e-4$

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	-0.024	-0.024	58	0.000	58					1
0.05	0.050					296					1
0.20	0.200	0.164	-0.036	815	0.0 %	815					18
2.50	2.500	2.503	0.003	10262	0.0 %	10262					0
5.00	5.000	5.028	0.028	20460	0.0 %	20460					1
7.50	7.500	7.707	0.207	31281	0.0 %	31281					3
10.0	10.000	9.824	-0.176	39831	0.0 %	39831					2

LB109953

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0.0	58	-		0 ISM02.4	PPB	7/10/2020 14:29	Std
	0.2 S0.2	815	-		0.2 ISM02.4	PPB	7/10/2020 14:31	Std
	2.5 S2.5	10262	-		2.5 ISM02.4	PPB	7/10/2020 14:34	Std
	5 S5.0	20460	-		5 ISM02.4	PPB	7/10/2020 14:36	Std
	7.5 S7.5	31281	-		7.5 ISM02.4	PPB	7/10/2020 14:41	Std
	10 S10.0	39831	-		10 ISM02.4	PPB	7/10/2020 14:43	Std
ICV	ICV	16256	3.9866 -		ISM02.4	PPB	7/10/2020 14:47	SMPL
ICB	ICB	-106	-0.0645 -		ISM02.4	PPB	7/10/2020 14:50	SMPL
CCV077	CCV077	20201	4.9634 -		ISM02.4	PPB	7/10/2020 14:52	SMPL
CCB077	CCB077	-171	-0.0806 -		ISM02.4	PPB	7/10/2020 14:54	SMPL
PB130100BL	PBW100	40	-0.0284 -		ISM02.4	PPB	7/10/2020 14:57	SMPL
L3262-01	MBE505	94	-0.015 -		ISM02.4	PPB	7/10/2020 15:04	SMPL
L3262-02	MBE505D	58	-0.0239 -		ISM02.4	PPB	7/10/2020 15:06	SMPL
L3262-03	MBE505S	4194	1.0001 -		ISM02.4	PPB	7/10/2020 15:08	SMPL
L3262-04	MBE506	92	-0.0155 -		ISM02.4	PPB	7/10/2020 15:10	SMPL
CCV078	CCV078	18699	4.5915 -		ISM02.4	PPB	7/10/2020 15:13	SMPL
CCB078	CCB078	-151	-0.0757 -		ISM02.4	PPB	7/10/2020 15:15	SMPL