


LB109957

7471B

INSTRUMENT ID: CV1

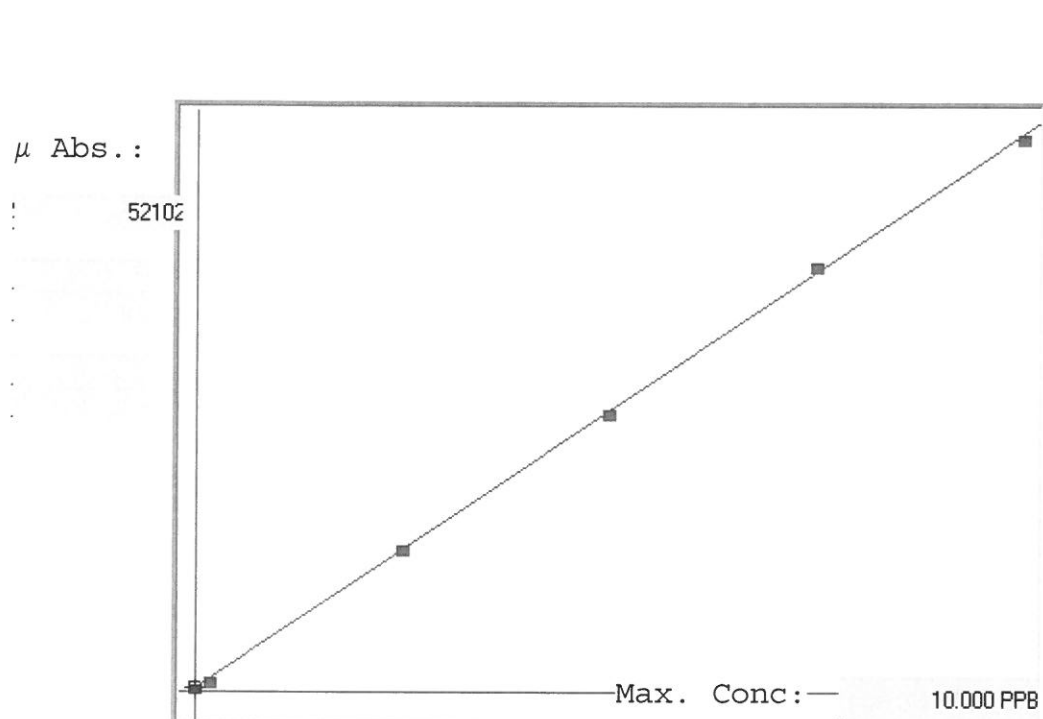

Linear

A= 0.0000e+000

B= 1.9138e-004

C= -5.3622e-002

Rho= 0.9998423

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.020	0.020	386	0.000	386				
0.2	0.200	0.146	-0.054	1045	0.0 %	1045				
2.5	2.500	2.527	0.027	13484	0.0 %	13484				
5.0	5.000	4.970	-0.030	26249	0.0 %	26249				
7.5	7.500	7.619	0.119	40089	0.0 %	40089				
10.0	10.000	9.918	-0.082	52102	0.0 %	52102				

LB109957 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 10 Jul 2020 15:33:10

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	386	-	0.0000	7471B	PPB	10 Jul 2020 15:34:35	S	Std
0.2 - 1	50.2	1045	-	0.2000	7471B	PPB	10 Jul 2020 15:36:52	S	Std
2.5 - 1	52.5	13484	-	2.5000	7471B	PPB	10 Jul 2020 15:39:09	S	Std
5.0 - 1	55	26249	-	5.0000	7471B	PPB	10 Jul 2020 15:41:26	S	Std
7.5 - 1	57.5	40089	-	7.5000	7471B	PPB	10 Jul 2020 15:43:42	S	Std
10.0 - 1	510	52102	-	10.0000	7471B	PPB	10 Jul 2020 15:48:40	S	Std
ICV23 - 1	ICV23	21803	4.1191	-	7471B	PPB	10 Jul 2020 15:51:37	U	SMPL
ICB23 - 1	ICB23	143	-0.0263	-	7471B	PPB	10 Jul 2020 15:53:52	U	SMPL
CCV79 - 1	CCV79	27145	5.1414	-	7471B	PPB	10 Jul 2020 15:56:08	U	SMPL
CCB79 - 1	CCB79	146	-0.0257	-	7471B	PPB	10 Jul 2020 15:58:23	U	SMPL
CRA - 1	CRA	1288	0.1929	-	7471B	PPB	10 Jul 2020 16:00:40	U	SMPL
HighStd - 1	HighStd	52288	9.9534	-	7471B	PPB	10 Jul 2020 16:02:55	U	SMPL
ChkStd - 1	ChkStd	37949	7.2091	-	7471B	PPB	10 Jul 2020 16:05:11	U	SMPL
PB130097BL - 1	PBS	222	-0.0111	-	7471B	PPB	10 Jul 2020 16:10:47	U	SMPL
PB130097BS - 1	LCSS	22558	4.2636	-	7471B	PPB	10 Jul 2020 16:13:03	U	SMPL
L3184-01 - 1	EO-02-070920	20882	3.9428	-	7471B	PPB	10 Jul 2020 16:15:20	U	SMPL
L3255-02 - 1	CHRT-57	56265	10.7145	-	7471B	PPB	10 Jul 2020 16:17:38	U	SMPL
L3255-02DUP - 1	CHRT-57DUP	52081	9.9137	-	7471B	PPB	10 Jul 2020 16:19:56	U	SMPL
L3255-02MS - 1	CHRT-57MS	73719	14.0549	-	7471B	PPB	10 Jul 2020 16:22:19	U	SMPL
L3255-02MSD - 1	CHRT-57MSD	70752	13.4870	-	7471B	PPB	10 Jul 2020 16:24:38	U	SMPL
CCV80 - 1	CCV80	28377	5.3772	-	7471B	PPB	10 Jul 2020 16:31:38	U	SMPL
CCB80 - 1	CCB80	144	-0.0261	-	7471B	PPB	10 Jul 2020 16:33:52	U	SMPL
L3255-06 - 1	CHRT-58	4490	0.8057	-	7471B	PPB	10 Jul 2020 16:36:09	U	SMPL
L3255-08 - 1	RBR-07	4813	0.8675	-	7471B	PPB	10 Jul 2020 16:38:24	U	SMPL
L3255-10 - 1	CHRT-17	2333	0.3929	-	7471B	PPB	10 Jul 2020 16:40:41	U	SMPL
L3255-12 - 1	CHRT-31	2164	0.3605	-	7471B	PPB	10 Jul 2020 16:42:59	U	SMPL
L3257-02 - 1	MH1	18753	3.5354	-	7471B	PPB	10 Jul 2020 16:45:15	U	SMPL
L3257-04 - 1	MH2	29443	5.5812	-	7471B	PPB	10 Jul 2020 16:47:32	U	SMPL
L3258-01 - 1	20200414-1	7817	1.4424	-	7471B	PPB	10 Jul 2020 16:49:51	U	SMPL
L3259-01 - 1	T-2-DRUM	-259	-0.1032	-	7471B	PPB	10 Jul 2020 16:52:10	U	SMPL
L3255-02LX5 - 1		10109	1.8811	-	7471B	PPB	10 Jul 2020 16:54:30	U	SMPL
L3255-02A - 1		76187	14.5272	-	7471B	PPB	10 Jul 2020 16:56:46	U	SMPL
CCV81 - 1	CCV81	24071	4.5531	-	7471B	PPB	10 Jul 2020 16:59:04	U	SMPL
CCB81 - 1	CCB81	53	-0.0435	-	7471B	PPB	10 Jul 2020 17:01:27	U	SMPL
L3255-02DLX2 - 1		28215	5.3462	-	7471B	PPB	10 Jul 2020 17:03:45	U	SMPL
L3255-02DUPDLX2 - 1		25938	4.9104	-	7471B	PPB	10 Jul 2020 17:06:00	U	SMPL
L3255-02MSDLX2 - 1		37226	7.0708	-	7471B	PPB	10 Jul 2020 17:08:19	U	SMPL
L3255-02MSDDLX2 - 1		37422	7.1083	-	7471B	PPB	10 Jul 2020 17:10:36	U	SMPL
L3255-02LDLX10 - 1		4888	0.8819	-	7471B	PPB	10 Jul 2020 17:12:55	U	SMPL
L3255-02ADLX2 - 1		37589	7.1402	-	7471B	PPB	10 Jul 2020 17:15:16	U	SMPL
CCV82 - 1	CCV82	26303	4.9803	-	7471B	PPB	10 Jul 2020 17:17:32	U	SMPL
CCB82 - 1	CCB82	154	-0.0241	-	7471B	PPB	10 Jul 2020 17:19:51	U	SMPL