

LB109982

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : JK

Instrument ID : Konelab

7/13/2020 13:44

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.043	0.0	0.079	
ICB1	0.446	0.0	0.002	
CCV1	244.146	0.0	0.197	
CCB1	0.485	0.0	0.002	
PB130114BL	0.647	0.0	0.002	
PB130114BS	96.384	0.0	0.079	
LOWPB130114	10.212	0.0	0.010	
HIGHPB130114	489.922	0.0	0.393	
L3217-08	132.435	0.0	0.108	
L3217-08DUP	131.772	0.0	0.107	
L3217-10	97.121	0.0	0.079	
CCV2	261.162	0.0	0.210	
CCB2	0.311	0.0	0.002	

N	13
Mean	120.083
SD	142.3991
CV%	118.58

Aquakem v. 7.2AQ1

Results from time period:

Mon Jul 13 13:41:01 2020

Mon Jul 13 13:44:25 2020

idh

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.2766	µg/l	7/13/2020 12:29:15	
5.OPPBCN	A	Total CN	P	4.8843	µg/l	7/13/2020 12:29:16	
10PPBCN	A	Total CN	P	9.9455	µg/l	7/13/2020 12:29:17	
50PPBCN	A	Total CN	P	49.3385	µg/l	7/13/2020 12:29:18	
100PPBCN	A	Total CN	P	99.5998	µg/l	7/13/2020 12:29:19	
250PPBCN	A	Total CN	P	252.7199	µg/l	7/13/2020 12:29:20	
500PPBCN	A	Total CN	P	498.7885	µg/l	7/13/2020 12:29:21	
ICV1	S	Total CN	P	96.0433	µg/l	7/13/2020 13:41:01	
ICB1	S	Total CN	P	0.4455	µg/l	7/13/2020 13:41:02	
CCV1	S	Total CN	P	244.1455	µg/l	7/13/2020 13:41:03	
CCB1	S	Total CN	P	0.485	µg/l	7/13/2020 13:41:04	
PB130114BL	S	Total CN	P	0.6465	µg/l	7/13/2020 13:41:05	
PB130114BS	S	Total CN	P	96.3835	µg/l	7/13/2020 13:41:06	
LOWPB130114	S	Total CN	P	10.2125	µg/l	7/13/2020 13:41:07	
HIGHPB130114	S	Total CN	P	489.9216	µg/l	7/13/2020 13:41:08	
L3217-08	S	Total CN	P	132.4346	µg/l	7/13/2020 13:41:09	
L3217-08DUP	S	Total CN	P	131.7719	µg/l	7/13/2020 13:41:10	
L3217-10	S	Total CN	P	97.1207	µg/l	7/13/2020 13:41:11	
CCV2	S	Total CN	P	261.1623	µg/l	7/13/2020 13:44:24	
CCB2	S	Total CN	P	0.3112	µg/l	7/13/2020 13:44:25	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DL

Instrument ID : Konelab

7/13/2020 13:01


Test Total CN

Accepted 7/13/2020 12:29

Factor 1254
Bias 0.002

Coeff. of det. 0.999954

Errors

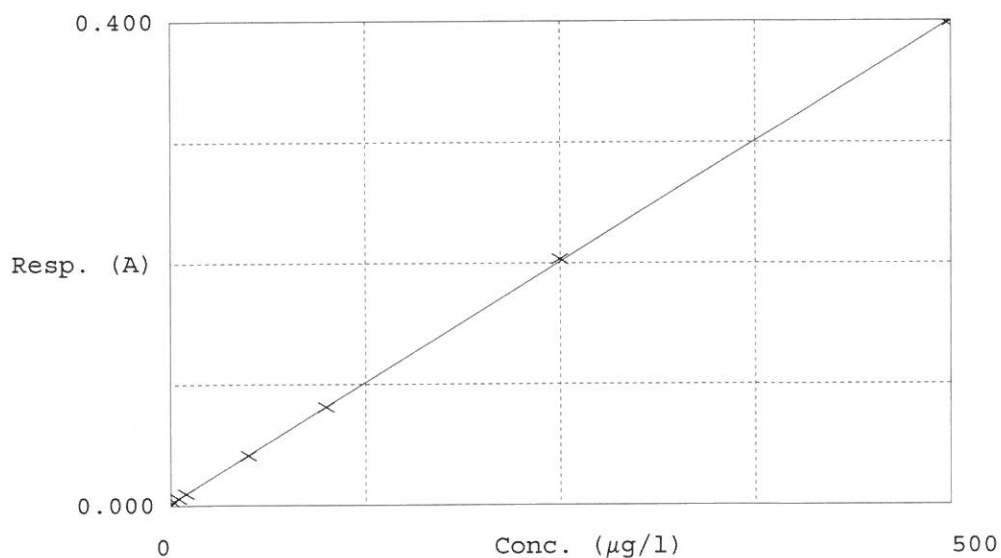

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.2766	0.0000	
2	5.0PPBCN	0.006	4.8843	5.0000	
3	10PPBCN	0.010	9.9455	10.0000	
4	50PPBCN	0.041	49.3385	50.0000	
5	100PPBCN	0.081	99.5998	100.0000	
6	250PPBCN	0.203	252.7199	250.0000	
7	500PPBCN	0.400	498.7885	500.0000	