


LB110029

7471B

INSTRUMENT ID: CV1

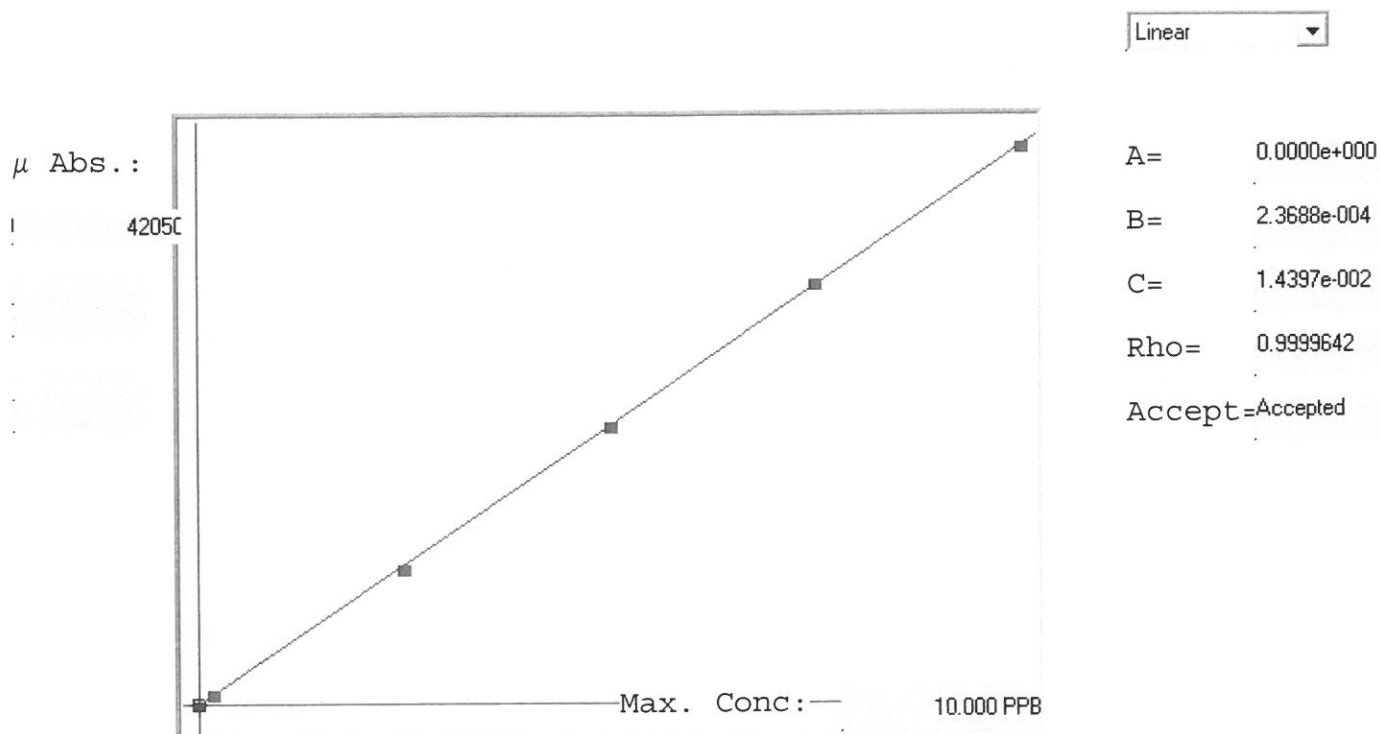

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.024	0.024	39	0.000	39				
0.2	0.200	0.201	0.001	789	0.0 %	789				
2.5	2.500	2.451	-0.049	10285	0.0 %	10285				
5.0	5.000	5.001	0.001	21053	0.0 %	21053				
7.5	7.500	7.548	0.048	31801	0.0 %	31801				
10.0	10.000	9.975	-0.025	42050	0.0 %	42050				

LB110029 INSTRUMENT ID : CV1

Method: 7471B	Operator: Admin	Date of Analysis: 15 Jul 2020 12:06:43				
Sample ID	Extended ID	µ Abs.	Conc.	Stnd ConcMethod	Units	Date Type Type
0.0 - 1	50	39	-	0.00007471B	PPB	15 Jul 2020 12:10:39 S Std
0.2 - 1	50.2	789	-	0.20007471B	PPB	15 Jul 2020 12:12:57 S Std
2.5 - 1	52.5	10285	-	2.50007471B	PPB	15 Jul 2020 12:15:14 S Std
5.0 - 1	55	21053	-	5.00007471B	PPB	15 Jul 2020 12:17:31 S Std
7.5 - 1	57.5	31801	-	7.50007471B	PPB	15 Jul 2020 12:22:20 S Std
10.0 - 1	50	42050	-	10.00007471B	PPB	15 Jul 2020 12:27:13 S Std
ICV29 - 1	ICV29	16487	3.9199	-7471B	PPB	15 Jul 2020 12:36:33 U SMPL
ICB29 - 1	ICB29	-155	-0.0223	-7471B	PPB	15 Jul 2020 12:38:48 U SMPL
CCV01 - 1	CCV01	21895	5.2009	-7471B	PPB	15 Jul 2020 12:41:04 U SMPL
CCB01 - 1	CCB01	-177	-0.0275	-7471B	PPB	15 Jul 2020 12:43:19 U SMPL
CRA - 1	CRA	764	0.1954	-7471B	PPB	15 Jul 2020 12:45:37 U SMPL
HighStd - 1	HighStd	42818	10.1573	-7471B	PPB	15 Jul 2020 12:47:52 U SMPL
ChkStd - 1	ChkStd	31703	7.5243	-7471B	PPB	15 Jul 2020 12:50:07 U SMPL
PB130221BL - 1	PBS	-146	-0.0202	-7471B	PPB	15 Jul 2020 12:52:26 U SMPL
PB130221BS - 1	LCSS	17379	4.1312	-7471B	PPB	15 Jul 2020 12:54:44 U SMPL
L3183-06 - 1	OK-01-071420	6352	1.5191	-7471B	PPB	15 Jul 2020 12:57:01 U SMPL
L3187-05 - 1	SU-03-071420	2969	0.7177	-7471B	PPB	15 Jul 2020 12:59:19 U SMPL
L3187-05DUP - 1	SU-03-071420DUP	3568	0.8596	-7471B	PPB	15 Jul 2020 13:03:32 U SMPL
L3187-05MS - 1	SU-03-071420MS	20015	4.7556	-7471B	PPB	15 Jul 2020 13:05:48 U SMPL
L3187-05MSD - 1	SU-03-071420MSD	19564	4.6488	-7471B	PPB	15 Jul 2020 13:08:06 U SMPL
CCV02 - 1	CCV02	21368	5.0761	-7471B	PPB	15 Jul 2020 13:10:23 U SMPL
CCB02 - 1	CCB02	-259	-0.0470	-7471B	PPB	15 Jul 2020 13:12:41 U SMPL
L3188-07 - 1	TR-05-071420	2948	0.7127	-7471B	PPB	15 Jul 2020 13:14:58 U SMPL
L3288-01 - 1	BS-DRUM	1219	0.3032	-7471B	PPB	15 Jul 2020 13:17:14 U SMPL
L3289-02 - 1	IRON-1	7340	1.7531	-7471B	PPB	15 Jul 2020 13:19:31 U SMPL
L3289-07 - 1	IRON-2	36522	8.6658	-7471B	PPB	15 Jul 2020 13:21:49 U SMPL
L3300-03 - 1	TP-8A-S	8423	2.0097	-7471B	PPB	15 Jul 2020 13:24:06 U SMPL
L3300-07 - 1	TP-8A-D	3831	0.9219	-7471B	PPB	15 Jul 2020 13:26:25 U SMPL
L3301-01 - 1	CARLSTADT-SAMPLE-2020	5675	1.3587	-7471B	PPB	15 Jul 2020 13:28:43 U SMPL
L3302-01 - 1	FK-GF-03-013-A	8956	2.1359	-7471B	PPB	15 Jul 2020 13:39:10 U SMPL
L3302-03 - 1	FK-GF-03-013-B	7817	1.8661	-7471B	PPB	15 Jul 2020 13:41:26 U SMPL
L3303-01 - 1	FK-GF-03-014-A	7257	1.7335	-7471B	PPB	15 Jul 2020 13:43:44 U SMPL
CCV03 - 1	CCV03	21806	5.1799	-7471B	PPB	15 Jul 2020 13:46:02 U SMPL
CCB03 - 1	CCB03	-239	-0.0422	-7471B	PPB	15 Jul 2020 13:48:20 U SMPL
L3303-03 - 1	FK-GF-03-014-B	8266	1.9725	-7471B	PPB	15 Jul 2020 13:50:37 U SMPL
L3304-01 - 1	FK-GF-02-058-A	13724	3.2654	-7471B	PPB	15 Jul 2020 13:52:52 U SMPL
L3304-03 - 1	FK-GF-02-058-B	10305	2.4555	-7471B	PPB	15 Jul 2020 13:55:10 U SMPL
L3305-01 - 1	FK-GF-02-057-A	12063	2.8719	-7471B	PPB	15 Jul 2020 13:57:28 U SMPL
L3305-03 - 1	FK-GF-02-057-B	10218	2.4349	-7471B	PPB	15 Jul 2020 13:59:45 U SMPL
L3187-05LX5 - 1		249	0.0734	-7471B	PPB	15 Jul 2020 14:02:03 U SMPL
L3187-05A - 1		19221	4.5675	-7471B	PPB	15 Jul 2020 14:04:20 U SMPL
CCV04 - 1	CCV04	21858	5.1922	-7471B	PPB	15 Jul 2020 14:06:37 U SMPL
CCB04 - 1	CCB04	-185	-0.0294	-7471B	PPB	15 Jul 2020 14:08:56 U SMPL