


LB110051

7470A

INSTRUMENT ID: CV1

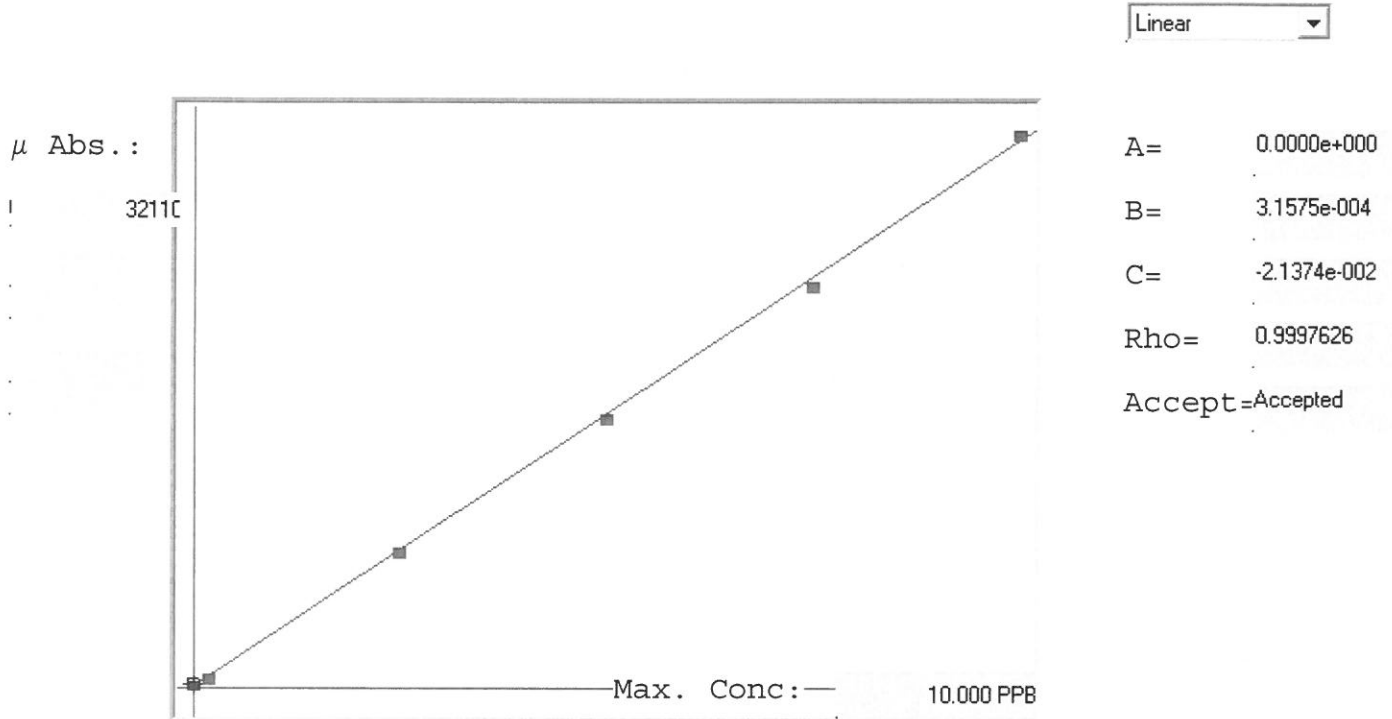

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.079	0.079	318	0.000	318				
0.2	0.200	0.184	-0.016	652	0.0 %	652				
2.5	2.500	2.494	-0.006	7967	0.0 %	7967				
5.0	5.000	4.953	-0.047	15753	0.0 %	15753				
7.5	7.500	7.372	-0.128	23417	0.0 %	23417				
10.0	10.000	10.117	0.117	32110	0.0 %	32110				

LB110051 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 Jul 2020 12:06:45

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	318	-	0.00007470A	PPB		16 Jul 2020 12:09:48	S	Std
0.2 - 1	50.2	652	-	0.20007470A	PPB		16 Jul 2020 12:11:55	S	Std
2.5 - 1	52.5	7967	-	2.50007470A	PPB		16 Jul 2020 12:14:03	S	Std
5.0 - 1	55	15753	-	5.00007470A	PPB		16 Jul 2020 12:16:11	S	Std
7.5 - 1	57.5	23417	-	7.50007470A	PPB		16 Jul 2020 12:18:18	S	Std
10.0 - 1	510	32110	-	10.00007470A	PPB		16 Jul 2020 12:25:21	S	Std
ICV30 - 1	ICV30	11966	3.7568	-7470A	PPB		16 Jul 2020 12:28:03	U	SMPL
ICB30 - 1	ICB30	-22	-0.0283	-7470A	PPB		16 Jul 2020 12:30:08	U	SMPL
CCV07 - 1	CCV07	15623	4.9115	-7470A	PPB		16 Jul 2020 12:32:14	U	SMPL
CCB07 - 1	CCB07	-8	-0.0239	-7470A	PPB		16 Jul 2020 12:34:20	U	SMPL
CRA - 1	CRA	584	0.1630	-7470A	PPB		16 Jul 2020 12:41:08	U	SMPL
HighStd - 1	HighStd	31906	10.0528	-7470A	PPB		16 Jul 2020 12:43:14	U	SMPL
ChkStd - 1	ChkStd	22395	7.0498	-7470A	PPB		16 Jul 2020 12:45:20	U	SMPL
PB130234BL - 1	PBW	20	-0.0151	-7470A	PPB		16 Jul 2020 12:50:01	U	SMPL
PB130234BS - 1	LCSW	12036	3.7790	-7470A	PPB		16 Jul 2020 12:52:07	U	SMPL
L3183-10 - 1	OK-01-071420	-123	-0.0602	-7470A	PPB		16 Jul 2020 12:54:15	U	SMPL
L3183-10DUP - 1	OK-01-071420DUP	34	-0.0106	-7470A	PPB		16 Jul 2020 12:56:22	U	SMPL
L3183-10MS - 1	OK-01-071420MS	11285	3.5418	-7470A	PPB		16 Jul 2020 12:58:30	U	SMPL
L3183-10MSD - 1	OK-01-071420MSD	11901	3.7363	-7470A	PPB		16 Jul 2020 13:00:37	U	SMPL
L3187-08 - 1	SU-03-071420	-87	-0.0488	-7470A	PPB		16 Jul 2020 13:02:43	U	SMPL
CCV08 - 1	CCV08	16094	5.0603	-7470A	PPB		16 Jul 2020 13:04:49	U	SMPL
CCB08 - 1	CCB08	-42	-0.0346	-7470A	PPB		16 Jul 2020 13:06:55	U	SMPL
L3188-10 - 1	TR-05-071420	89	0.0067	-7470A	PPB		16 Jul 2020 13:09:02	U	SMPL
L3289-03 - 1	IRON-1	148	0.0254	-7470A	PPB		16 Jul 2020 13:11:08	U	SMPL
L3289-08 - 1	IRON-2	166	0.0310	-7470A	PPB		16 Jul 2020 13:13:14	U	SMPL
L3300-04 - 1	TP-8A-S	195	0.0402	-7470A	PPB		16 Jul 2020 13:15:20	U	SMPL
L3300-08 - 1	TP-8A-D	140	0.0228	-7470A	PPB		16 Jul 2020 13:17:27	U	SMPL
PB130235BL - 1	PBW	180	0.0355	-7470A	PPB		16 Jul 2020 13:19:34	U	SMPL
PB130235BS - 1	LCSW	12739	4.0009	-7470A	PPB		16 Jul 2020 13:21:41	U	SMPL
L3258-02 - 1	20200415-FIELD-BLANK	-69	-0.0432	-7470A	PPB		16 Jul 2020 13:23:49	U	SMPL
CCV09 - 1	CCV09	16176	5.0861	-7470A	PPB		16 Jul 2020 13:25:56	U	SMPL
CCB09 - 1	CCB09	7	-0.0192	-7470A	PPB		16 Jul 2020 13:28:03	U	SMPL
PB130234TB - 1	PB130206TB	75	0.0023	-7470A	PPB		16 Jul 2020 13:30:10	U	SMPL
L3183-10LX5 - 1		217	0.0471	-7470A	PPB		16 Jul 2020 13:32:17	U	SMPL
L3183-10A - 1		12027	3.7761	-7470A	PPB		16 Jul 2020 13:34:23	U	SMPL
CCV10 - 1	CCV10	15710	4.9390	-7470A	PPB		16 Jul 2020 13:36:29	U	SMPL
CCB10 - 1	CCB10	-50	-0.0372	-7470A	PPB		16 Jul 2020 13:38:36	U	SMPL