


LB110116

7470A

INSTRUMENT ID: CV1

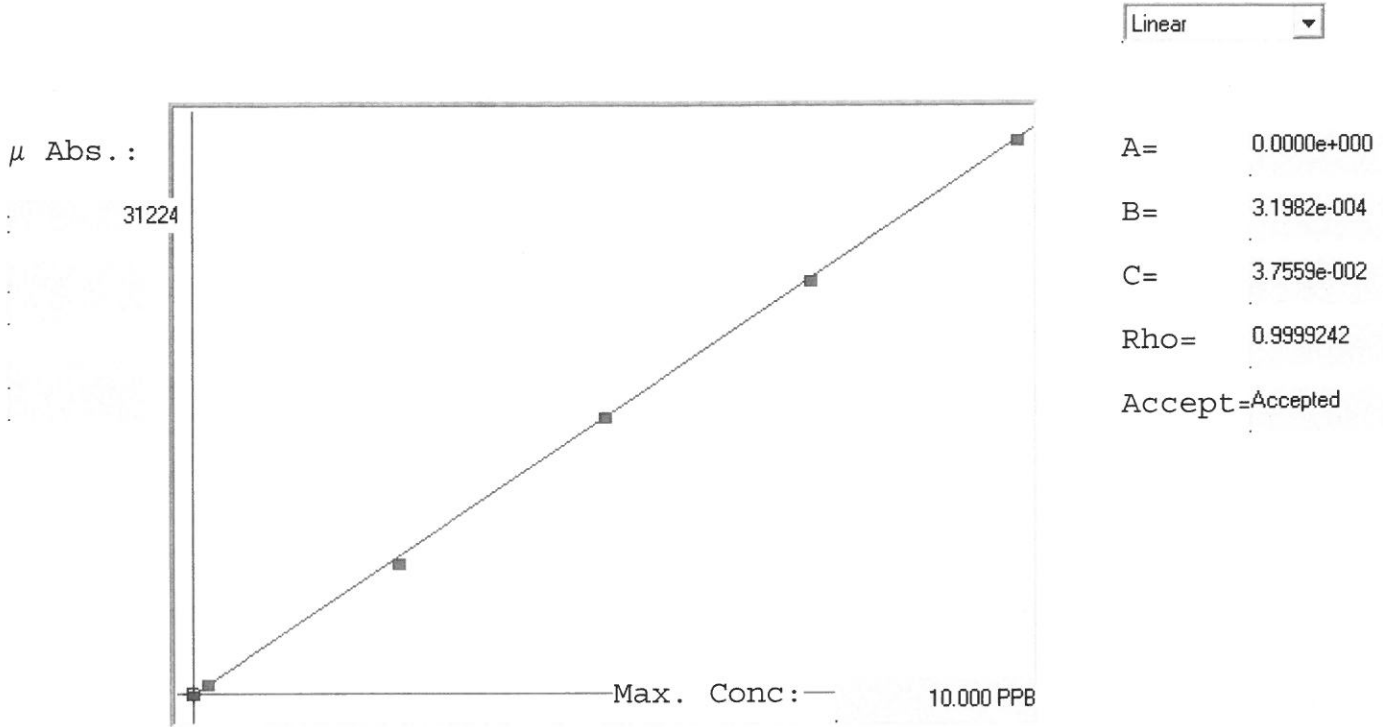

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.035	0.035	-7	0.000	-7				
0.2	0.200	0.220	0.020	570	0.0 %	570				
2.5	2.500	2.413	-0.087	7426	0.0 %	7426				
5.0	5.000	5.040	0.040	15640	0.0 %	15640				
7.5	7.500	7.469	-0.031	23236	0.0 %	23236				
10.0	10.000	10.024	0.024	31224	0.0 %	31224				

LB110116 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 21 Jul 2020 12:00:20

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-7	-	0.0000	7470A	PPB	21 Jul 2020 12:03:03	S	Std
0.2 - 1	50.2	570	-	0.2000	7470A	PPB	21 Jul 2020 12:05:11	S	Std
2.5 - 1	52.5	7426	-	2.5000	7470A	PPB	21 Jul 2020 12:07:19	S	Std
5.0 - 1	55	15640	-	5.0000	7470A	PPB	21 Jul 2020 12:09:26	S	Std
7.5 - 1	57.5	23236	-	7.5000	7470A	PPB	21 Jul 2020 12:11:33	S	Std
10.0 - 1	510	31224	-	10.0000	7470A	PPB	21 Jul 2020 12:13:40	S	Std
ICV34 - 1	ICV34	12417	4.0088	-7470A	PPB	21 Jul 2020 12:16:17	U	SMPL	
ICB34 - 1	ICB34	-368	-0.0801	-7470A	PPB	21 Jul 2020 12:18:22	U	SMPL	
CCV24 - 1	CCV24	15819	5.0968	-7470A	PPB	21 Jul 2020 12:20:29	U	SMPL	
CCB24 - 1	CCB24	-369	-0.0805	-7470A	PPB	21 Jul 2020 12:22:35	U	SMPL	
CRA - 1	CRA	437	0.1773	-7470A	PPB	21 Jul 2020 12:24:41	U	SMPL	
HighStd - 1	HighStd	31686	10.1715	-7470A	PPB	21 Jul 2020 12:26:47	U	SMPL	
ChkStd - 1	ChkStd	22890	7.3583	-7470A	PPB	21 Jul 2020 12:28:53	U	SMPL	
PB130307BL - 1	PBW	-156	-0.0123	-7470A	PPB	21 Jul 2020 12:33:24	U	SMPL	
PB130307BS - 1	LCSW	12023	3.8828	-7470A	PPB	21 Jul 2020 12:35:30	U	SMPL	
L3188-16 - 1	TR-04-071620	-340	-0.0712	-7470A	PPB	21 Jul 2020 12:37:37	U	SMPL	
L3188-16DUP - 1	TR-04-071620DUP	-187	-0.0222	-7470A	PPB	21 Jul 2020 12:39:45	U	SMPL	
L3188-16MS - 1	TR-04-071620MS	12276	3.9637	-7470A	PPB	21 Jul 2020 12:41:52	U	SMPL	
L3188-16MSD - 1	TR-04-071620MSD	11854	3.8287	-7470A	PPB	21 Jul 2020 12:44:01	U	SMPL	
L3323-01 - 1	225	-378	-0.0833	-7470A	PPB	21 Jul 2020 12:46:07	U	SMPL	
CCV25 - 1	CCV25	16164	5.2072	-7470A	PPB	21 Jul 2020 12:48:15	U	SMPL	
CCB25 - 1	CCB25	-385	-0.0856	-7470A	PPB	21 Jul 2020 12:50:21	U	SMPL	
L3323-02 - 1	221	-189	-0.0229	-7470A	PPB	21 Jul 2020 12:52:28	U	SMPL	
L3324-03 - 1	CHRT-26948	-139	-0.0069	-7470A	PPB	21 Jul 2020 12:54:34	U	SMPL	
L3335-04 - 1	TP-12-S	-117	0.0001	-7470A	PPB	21 Jul 2020 12:56:41	U	SMPL	
L3335-08 - 1	TP-11-S	-97	0.0065	-7470A	PPB	21 Jul 2020 12:58:48	U	SMPL	
L3335-12 - 1	TP-11-D	-37	0.0257	-7470A	PPB	21 Jul 2020 13:00:55	U	SMPL	
PB130308BL - 1	PBW	-89	0.0091	-7470A	PPB	21 Jul 2020 13:03:02	U	SMPL	
PB130308BS - 1	LCSW	11767	3.8009	-7470A	PPB	21 Jul 2020 13:05:09	U	SMPL	
L3323-03 - 1	223-224	-276	-0.0507	-7470A	PPB	21 Jul 2020 13:07:17	U	SMPL	
L3323-05 - 1	219-220	-22	0.0305	-7470A	PPB	21 Jul 2020 13:09:25	U	SMPL	
L3324-05 - 1	TOTE-50-DIAZ	-95	0.0072	-7470A	PPB	21 Jul 2020 13:11:31	U	SMPL	
CCV26 - 1	CCV26	15693	5.0565	-7470A	PPB	21 Jul 2020 13:13:37	U	SMPL	
CCB26 - 1	CCB26	-304	-0.0597	-7470A	PPB	21 Jul 2020 13:15:44	U	SMPL	
L3324-05DUP - 1	TOTE-50-DIAZDUP	-114	0.0011	-7470A	PPB	21 Jul 2020 13:17:50	U	SMPL	
L3324-05MS - 1	TOTE-50-DIAZMS	12038	3.8876	-7470A	PPB	21 Jul 2020 13:19:56	U	SMPL	
L3324-05MSD - 1	TOTE-50-DIAZMSD	13432	4.3334	-7470A	PPB	21 Jul 2020 13:22:03	U	SMPL	
PB130309BL - 1	PBW	-342	-0.0718	-7470A	PPB	21 Jul 2020 13:24:11	U	SMPL	
PB130309BS - 1	LCSW	11341	3.6647	-7470A	PPB	21 Jul 2020 13:26:18	U	SMPL	
L3177-04 - 1	AU-05-071720	-325	-0.0664	-7470A	PPB	21 Jul 2020 13:28:25	U	SMPL	
L3177-04DUP - 1	AU-05-071720DUP	-163	-0.0146	-7470A	PPB	21 Jul 2020 13:30:34	U	SMPL	
L3177-04MS - 1	AU-05-071720MS	12157	3.9256	-7470A	PPB	21 Jul 2020 13:32:41	U	SMPL	
L3177-04MSD - 1	AU-05-071720MSD	11163	3.6077	-7470A	PPB	21 Jul 2020 13:34:49	U	SMPL	
L3182-05 - 1	NB-08-071720	-278	-0.0514	-7470A	PPB	21 Jul 2020 13:36:56	U	SMPL	
CCV27 - 1	CCV27	15964	5.1432	-7470A	PPB	21 Jul 2020 13:39:02	U	SMPL	
CCB27 - 1	CCB27	-394	-0.0885	-7470A	PPB	21 Jul 2020 13:41:08	U	SMPL	
L3344-04 - 1	TP-15-S	-165	-0.0152	-7470A	PPB	21 Jul 2020 13:43:16	U	SMPL	
L3344-08 - 1	TP-14-S	-106	0.0037	-7470A	PPB	21 Jul 2020 13:45:22	U	SMPL	
L3344-12 - 1	TP-14-D	-79	0.0123	-7470A	PPB	21 Jul 2020 13:47:29	U	SMPL	
PB130319BL - 1	PBW	-42	0.0241	-7470A	PPB	21 Jul 2020 13:49:35	U	SMPL	
PB130319BS - 1	LCSW	11545	3.7299	-7470A	PPB	21 Jul 2020 13:51:42	U	SMPL	
L3334-01 - 1	I-OC-4	1423	0.4927	-7470A	PPB	21 Jul 2020 13:53:49	U	SMPL	
L3334-01DUP - 1	I-OC-4DUP	1195	0.4197	-7470A	PPB	21 Jul 2020 13:55:56	U	SMPL	
L3334-01MS - 1	I-OC-4MS	13278	4.2842	-7470A	PPB	21 Jul 2020 13:58:06	U	SMPL	
L3334-01MSD - 1	I-OC-4MSD	12832	4.1415	-7470A	PPB	21 Jul 2020 14:00:14	U	SMPL	
L3334-05 - 1	I-R-4	2407	0.8074	-7470A	PPB	21 Jul 2020 14:02:22	U	SMPL	
CCV28 - 1	CCV28	15131	4.8768	-7470A	PPB	21 Jul 2020 14:04:30	U	SMPL	
CCB28 - 1	CCB28	-225	-0.0344	-7470A	PPB	21 Jul 2020 14:06:37	U	SMPL	
L3334-06 - 1	E-R-4	1777	0.6059	-7470A	PPB	21 Jul 2020 14:08:43	U	SMPL	
PB130307TB - 1	PB130261TB	-152	-0.0111	-7470A	PPB	21 Jul 2020 14:10:50	U	SMPL	
PB130308TB - 1	PB130266TB	-52	0.0209	-7470A	PPB	21 Jul 2020 14:12:56	U	SMPL	
PB130309TB - 1	PB130291TB	-45	0.0232	-7470A	PPB	21 Jul 2020 14:15:02	U	SMPL	
L3188-16LX5 - 1		-10	0.0344	-7470A	PPB	21 Jul 2020 14:17:09	U	SMPL	
L3188-16A - 1		11607	3.7497	-7470A	PPB	21 Jul 2020 14:19:16	U	SMPL	
L3324-05LX5 - 1		-172	-0.0175	-7470A	PPB	21 Jul 2020 14:21:24	U	SMPL	
L3324-05A - 1		12535	4.0465	-7470A	PPB	21 Jul 2020 14:23:32	U	SMPL	
L3177-04LX5 - 1		-239	-0.0389	-7470A	PPB	21 Jul 2020 14:25:40	U	SMPL	
L3177-04A - 1		11900	3.8435	-7470A	PPB	21 Jul 2020 14:27:47	U	SMPL	
CCV29 - 1	CCV29	15752	5.0754	-7470A	PPB	21 Jul 2020 14:29:54	U	SMPL	
CCB29 - 1	CCB29	-379	-0.0837	-7470A	PPB	21 Jul 2020 14:32:00	U	SMPL	
L3334-01LX5 - 1		-89	0.0091	-7470A	PPB	21 Jul 2020 14:34:08	U	SMPL	
L3334-01A - 1		14399	4.6427	-7470A	PPB	21 Jul 2020 14:36:14	U	SMPL	
CCV30 - 1	CCV30	15370	4.9532	-7470A	PPB	21 Jul 2020 14:38:21	U	SMPL	
CCB30 - 1	CCB30	-335	-0.0696	-7470A	PPB	21 Jul 2020 14:40:30	U	SMPL	