


LB110130

7470A

INSTRUMENT ID: CV1

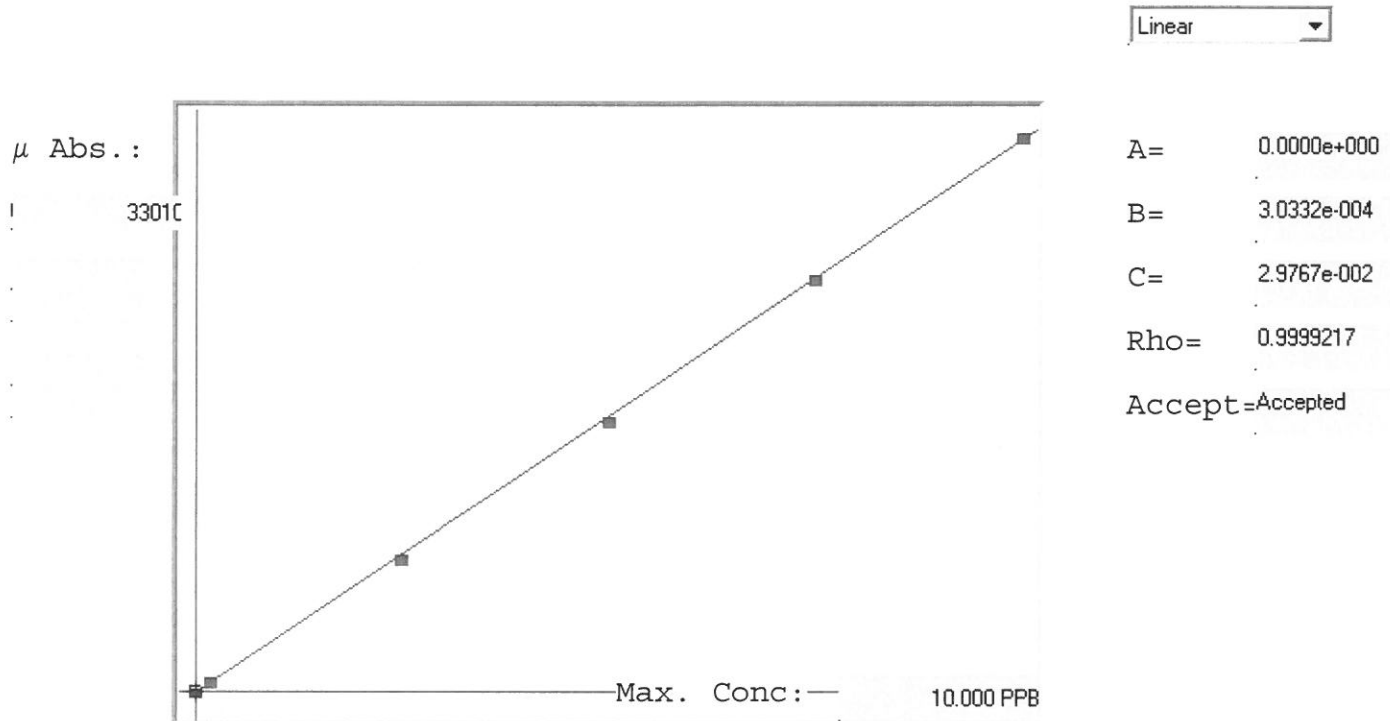

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.046	0.046	53	0.000	53				
0.2	0.200	0.227	0.027	650	0.0 %	650				
2.5	2.500	2.454	-0.046	7994	0.0 %	7994				
5.0	5.000	4.922	-0.078	16130	0.0 %	16130				
7.5	7.500	7.508	0.008	24656	0.0 %	24656				
10.0	10.000	10.042	0.042	33010	0.0 %	33010				

LB110130 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 22 Jul 2020 10:17:12					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	53	-	0.0000	7470A	PPB	22 Jul 2020 10:26:13	S	Std
0.2 - 1	50.2	650	-	0.2000	7470A	PPB	22 Jul 2020 10:28:20	S	Std
2.5 - 1	52.5	7994	-	2.5000	7470A	PPB	22 Jul 2020 10:30:28	S	Std
5.0 - 1	55	16130	-	5.0000	7470A	PPB	22 Jul 2020 10:32:35	S	Std
7.5 - 1	57.5	24656	-	7.5000	7470A	PPB	22 Jul 2020 10:34:42	S	Std
10.0 - 1	50	33010	-	10.0000	7470A	PPB	22 Jul 2020 10:36:49	S	Std
ICV35 - 1	ICV35	13525	4.1321	-	7470A	PPB	22 Jul 2020 10:39:27	U	SMPL
ICB35 - 1	ICB35	-199	-0.0306	-	7470A	PPB	22 Jul 2020 10:41:33	U	SMPL
CCV35 - 1	CCV35	16041	4.8952	-	7470A	PPB	22 Jul 2020 10:43:39	U	SMPL
CCB35 - 1	CCB35	-188	-0.0273	-	7470A	PPB	22 Jul 2020 10:45:45	U	SMPL
CRA - 1	CRA	581	0.2060	-	7470A	PPB	22 Jul 2020 10:47:51	U	SMPL
HighStd - 1	HighStd	33501	10.1911	-	7470A	PPB	22 Jul 2020 10:49:56	U	SMPL
ChkStd - 1	ChkStd	22776	6.9381	-	7470A	PPB	22 Jul 2020 10:52:02	U	SMPL
PB130352BL - 1	PBW	-338	-0.0728	-	7470A	PPB	22 Jul 2020 10:54:11	U	SMPL
PB130352BS - 1	LCSW	12219	3.7360	-	7470A	PPB	22 Jul 2020 10:56:19	U	SMPL
L3184-17 - 1	EO-03-072020	-201	-0.0312	-	7470A	PPB	22 Jul 2020 10:58:26	U	SMPL
L3184-17DUP - 1	EO-03-072020DUP	-65	0.0101	-	7470A	PPB	22 Jul 2020 11:00:34	U	SMPL
L3184-17MS - 1	EO-03-072020MS	12652	3.8673	-	7470A	PPB	22 Jul 2020 11:02:41	U	SMPL
L3184-17MSD - 1	EO-03-072020MSD	13059	3.9908	-	7470A	PPB	22 Jul 2020 11:04:49	U	SMPL
L3352-02 - 1	HS-01	-144	-0.0139	-	7470A	PPB	22 Jul 2020 11:06:56	U	SMPL
CCV36 - 1	CCV36	16508	5.0369	-	7470A	PPB	22 Jul 2020 11:09:04	U	SMPL
CCB36 - 1	CCB36	-251	-0.0464	-	7470A	PPB	22 Jul 2020 11:11:10	U	SMPL
PB130353BL - 1	PBW	53	0.0458	-	7470A	PPB	22 Jul 2020 11:13:18	U	SMPL
PB130353BS - 1	LCSW	12682	3.8764	-	7470A	PPB	22 Jul 2020 11:15:23	U	SMPL
L3368-02 - 1	20200421-SITE-WATER	158	0.0777	-	7470A	PPB	22 Jul 2020 11:17:29	U	SMPL
L3368-02DUP - 1	20200421-SITE-WATERDUP	145	0.0737	-	7470A	PPB	22 Jul 2020 11:19:36	U	SMPL
L3368-02MS - 1	20200421-SITE-WATERMS	14334	4.3775	-	7470A	PPB	22 Jul 2020 11:25:06	U	SMPL
L3368-02MSD - 1	20200421-SITE-WATERMSD	14513	4.4318	-	7470A	PPB	22 Jul 2020 11:27:12	U	SMPL
L3368-03 - 1	20200422-FIELD-BLANK	-343	-0.0743	-	7470A	PPB	22 Jul 2020 11:29:20	U	SMPL
CCV37 - 1	CCV37	16356	4.9908	-	7470A	PPB	22 Jul 2020 11:31:29	U	SMPL
CCB37 - 1	CCB37	-296	-0.0600	-	7470A	PPB	22 Jul 2020 11:33:37	U	SMPL
PB130352TB - 1	PB130328TB	-50	0.0146	-	7470A	PPB	22 Jul 2020 11:37:59	U	SMPL
L3184-17LX5 - 1		-33	0.0198	-	7470A	PPB	22 Jul 2020 11:40:04	U	SMPL
L3184-17A - 1		12598	3.8509	-	7470A	PPB	22 Jul 2020 11:42:11	U	SMPL
L3368-02LX5 - 1		-164	-0.0200	-	7470A	PPB	22 Jul 2020 11:44:17	U	SMPL
L3368-02A - 1		15157	4.6271	-	7470A	PPB	22 Jul 2020 11:46:23	U	SMPL
CCV38 - 1	CCV38	16282	4.9683	-	7470A	PPB	22 Jul 2020 11:48:29	U	SMPL
CCB38 - 1	CCB38	-342	-0.0740	-	7470A	PPB	22 Jul 2020 11:50:37	U	SMPL