


LB110164

7471B

INSTRUMENT ID : CV2

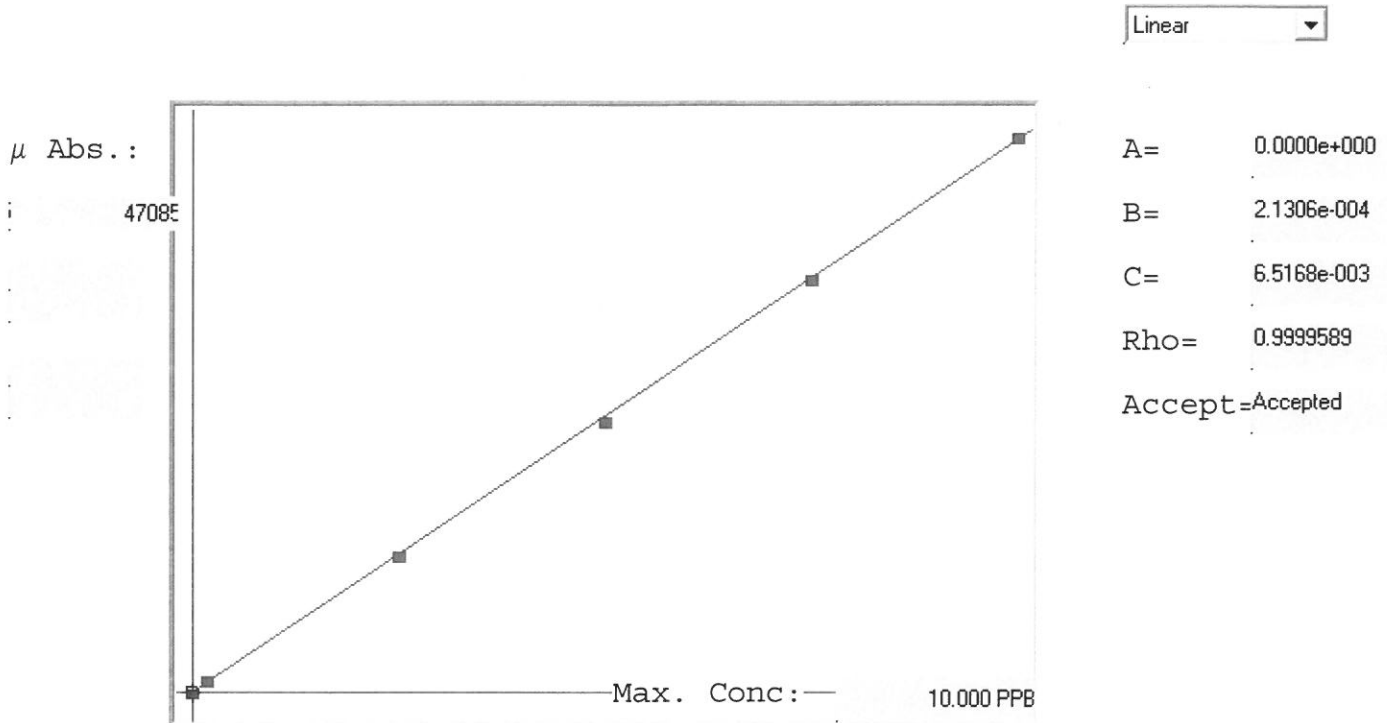

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.014	0.014	37	0.000	37				
0.2	0.200	0.221	0.021	1008	0.0 %	1008				
2.5	2.500	2.501	0.001	11710	0.0 %	11710				
5.0	5.000	4.933	-0.067	23122	0.0 %	23122				
7.5	7.500	7.491	-0.009	35130	0.0 %	35130				
10.0	10.000	10.039	0.039	47085	0.0 %	47085				

LB110164 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 Jul 2020 14:25:28

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	37	-	0.00007471B	PPB	23 Jul 2020 14:26:37	S	Std
0.2 - 1	50.2	1008	-	0.20007471B	PPB	23 Jul 2020 14:28:55	S	Std
2.5 - 1	52.5	11710	-	2.50007471B	PPB	23 Jul 2020 14:31:12	S	Std
5.0 - 1	55	23122	-	5.00007471B	PPB	23 Jul 2020 14:33:28	S	Std
7.5 - 1	57.5	35130	-	7.50007471B	PPB	23 Jul 2020 14:35:45	S	Std
10.0 - 1	510	47085	-	10.00007471B	PPB	23 Jul 2020 14:38:00	S	Std
ICV38 - 1	ICV38	18018	3.8455	-7471B	PPB	23 Jul 2020 14:41:54	U	SMPL
ICB38 - 1	ICB38	-147	-0.0248	-7471B	PPB	23 Jul 2020 14:44:09	U	SMPL
CCV51 - 1	CCV51	23911	5.1010	-7471B	PPB	23 Jul 2020 14:46:25	U	SMPL
CCB51 - 1	CCB51	-132	-0.0216	-7471B	PPB	23 Jul 2020 14:48:40	U	SMPL
CRA - 1	CRA	997	0.2189	-7471B	PPB	23 Jul 2020 14:50:56	U	SMPL
HighStd - 1	HighStd	47689	10.1672	-7471B	PPB	23 Jul 2020 14:53:11	U	SMPL
ChkStd - 1	ChkStd	33461	7.1358	-7471B	PPB	23 Jul 2020 14:55:26	U	SMPL
PB130414BL - 1	PBS	-157	-0.0269	-7471B	PPB	23 Jul 2020 14:57:44	U	SMPL
PB130414BS - 1	LCSS	16903	3.6079	-7471B	PPB	23 Jul 2020 15:00:02	U	SMPL
L3377-03 - 1	PAINT-COMP	128476	27.3799	-7471B	PPB	23 Jul 2020 15:02:18	U	SMPL
L3378-14 - 1	DRUM-COMP	3819	0.8202	-7471B	PPB	23 Jul 2020 15:04:36	U	SMPL
L3379-01 - 1	ETGI-361	44747	9.5404	-7471B	PPB	23 Jul 2020 15:07:11	U	SMPL
L3380-01 - 1	VNJ-221	2123	0.4588	-7471B	PPB	23 Jul 2020 15:14:21	U	SMPL
L3380-01DUP - 1	VNJ-221DUP	1944	0.4207	-7471B	PPB	23 Jul 2020 15:16:37	U	SMPL
CCV52 - 1	CCV52	24440	5.2137	-7471B	PPB	23 Jul 2020 15:18:53	U	SMPL
CCB52 - 1	CCB52	-183	-0.0325	-7471B	PPB	23 Jul 2020 15:21:09	U	SMPL
L3380-01MS - 1	VNJ-221MS	19015	4.0579	-7471B	PPB	23 Jul 2020 15:23:25	U	SMPL
L3380-01MSD - 1	VNJ-221MSD	20415	4.3562	-7471B	PPB	23 Jul 2020 15:25:40	U	SMPL
L3380-03 - 1	VNJ-241	3548	0.7625	-7471B	PPB	23 Jul 2020 15:27:58	U	SMPL
L3380-05 - 1	VNJ-242	2672	0.5758	-7471B	PPB	23 Jul 2020 15:30:16	U	SMPL
L3381-01 - 1	357-GRID-A4-A6	32031	6.8311	-7471B	PPB	23 Jul 2020 15:32:34	U	SMPL
L3381-04 - 1	347-GRID-B1-B2	31567	6.7322	-7471B	PPB	23 Jul 2020 15:34:53	U	SMPL
L3381-07 - 1	364-GRID-A7-A8	74392	15.8566	-7471B	PPB	23 Jul 2020 15:37:12	U	SMPL
L3381-10 - 1	359-GRID-A1-A3	30179	6.4365	-7471B	PPB	23 Jul 2020 15:39:32	U	SMPL
L3381-13 - 1	339-GRID-B3-B4	1684	0.3653	-7471B	PPB	23 Jul 2020 15:41:52	U	SMPL
L3381-16 - 1	365-GRID-B6-B8	6885	1.4734	-7471B	PPB	23 Jul 2020 15:44:11	U	SMPL
CCV53 - 1	CCV53	21564	4.6010	-7471B	PPB	23 Jul 2020 15:51:19	U	SMPL
CCB53 - 1	CCB53	-133	-0.0218	-7471B	PPB	23 Jul 2020 15:53:34	U	SMPL
L3381-19 - 1	VNJ-225-GRID-B5	8349	1.7854	-7471B	PPB	23 Jul 2020 15:55:51	U	SMPL
L3380-01LX5 - 1		68	0.0210	-7471B	PPB	23 Jul 2020 15:58:06	U	SMPL
L3380-01A - 1		20351	4.3425	-7471B	PPB	23 Jul 2020 16:00:24	U	SMPL
L3377-03DLX5 - 1		27974	5.9667	-7471B	PPB	23 Jul 2020 16:02:40	U	SMPL
L3381-07DLX5 - 1		14481	3.0919	-7471B	PPB	23 Jul 2020 16:04:58	U	SMPL
CCV54 - 1	CCV54	22350	4.7684	-7471B	PPB	23 Jul 2020 16:54:48	U	SMPL
CCB54 - 1	CCB54	-243	-0.0453	-7471B	PPB	23 Jul 2020 16:57:04	U	SMPL