

LB110214


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

33259

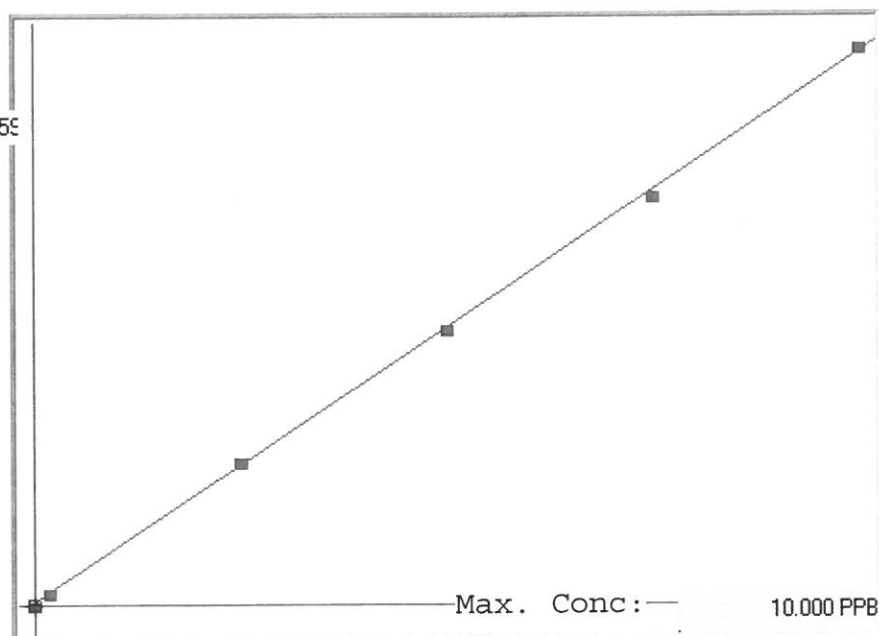

A= 0.0000e+000

B= 3.0381e-004

C= -3.8657e-002

Rho= 0.9998801

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.012	-0.012	89	0.000	89				
0.2	0.200	0.198	-0.002	778	0.0 %	778				
2.5	2.500	2.572	0.072	8594	0.0 %	8594				
5.0	5.000	4.971	-0.029	16488	0.0 %	16488				
7.5	7.500	7.405	-0.095	24501	0.0 %	24501				
10.0	10.000	10.066	0.066	33259	0.0 %	33259				

LB110214 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 27 Jul 2020 11:40:52					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	89	-	0.0000	7470A	PPB	27 Jul 2020 11:43:15	S	Std
0.2 - 1	50.2	778	-	0.2000	7470A	PPB	27 Jul 2020 11:45:23	S	Std
2.5 - 1	52.5	8594	-	2.5000	7470A	PPB	27 Jul 2020 11:47:31	S	Std
5.0 - 1	55	16488	-	5.0000	7470A	PPB	27 Jul 2020 11:49:39	S	Std
7.5 - 1	57.5	24501	-	7.5000	7470A	PPB	27 Jul 2020 11:51:46	S	Std
10.0 - 1	510	33259	-	10.0000	7470A	PPB	27 Jul 2020 11:53:53	S	Std
ICV42 - 1	ICV42	12750	3.8350	-	7470A	PPB	27 Jul 2020 11:57:06	U	SMPL
ICB42 - 1	ICB42	-4	-0.0399	-	7470A	PPB	27 Jul 2020 11:59:11	U	SMPL
CCV70 - 1	CCV70	16637	5.0159	-	7470A	PPB	27 Jul 2020 12:03:43	U	SMPL
CCB70 - 1	CCB70	6	-0.0368	-	7470A	PPB	27 Jul 2020 12:05:48	U	SMPL
CRA - 1	CRA	661	0.1622	-	7470A	PPB	27 Jul 2020 12:07:55	U	SMPL
HighStd - 1	HighStd	33396	10.1075	-	7470A	PPB	27 Jul 2020 12:10:00	U	SMPL
ChkStd - 1	ChkStd	22999	6.9488	-	7470A	PPB	27 Jul 2020 12:12:06	U	SMPL
PB130475BS - 1	LCSW	12157	3.6548	-	7470A	PPB	27 Jul 2020 12:16:24	U	SMPL
L3377-04 - 1	PAINT-COMP	-133	-0.0791	-	7470A	PPB	27 Jul 2020 12:18:31	U	SMPL
L3382-03 - 1	CTR-007	-29	-0.0475	-	7470A	PPB	27 Jul 2020 12:20:38	U	SMPL
L3382-03DUP - 1	CTR-007DUP	12	-0.0350	-	7470A	PPB	27 Jul 2020 12:22:46	U	SMPL
L3382-03MS - 1	CTR-007MS	14915	4.4927	-	7470A	PPB	27 Jul 2020 12:24:54	U	SMPL
L3382-03MSD - 1	CTR-007MSD	12878	3.8739	-	7470A	PPB	27 Jul 2020 12:27:00	U	SMPL
CCV71 - 1	CCV71	17418	5.2532	-	7470A	PPB	27 Jul 2020 12:31:34	U	SMPL
CCB71 - 1	CCB71	-134	-0.0794	-	7470A	PPB	27 Jul 2020 12:33:40	U	SMPL
L3382-07 - 1	CTR-020	-58	-0.0563	-	7470A	PPB	27 Jul 2020 12:35:47	U	SMPL
L3382-11 - 1	CTR-023	-3	-0.0396	-	7470A	PPB	27 Jul 2020 12:37:53	U	SMPL
L3382-15 - 1	CTR-005	17	-0.0335	-	7470A	PPB	27 Jul 2020 12:39:59	U	SMPL
L3382-19 - 1	CTR-011	45	-0.0250	-	7470A	PPB	27 Jul 2020 12:42:06	U	SMPL
L3382-23 - 1	CTR-024	45	-0.0250	-	7470A	PPB	27 Jul 2020 12:44:12	U	SMPL
L3383-03 - 1	CRT-013	60	-0.0204	-	7470A	PPB	27 Jul 2020 12:46:19	U	SMPL
L3383-07 - 1	CRT-018	65	-0.0189	-	7470A	PPB	27 Jul 2020 12:48:26	U	SMPL
L3383-11 - 1	CRT-009	63	-0.0195	-	7470A	PPB	27 Jul 2020 12:50:34	U	SMPL
L3383-15 - 1	CRT-022	53	-0.0226	-	7470A	PPB	27 Jul 2020 12:52:42	U	SMPL
L3383-19 - 1	CRT-008	81	-0.0140	-	7470A	PPB	27 Jul 2020 12:54:48	U	SMPL
CCV72 - 1	CCV72	16593	5.0025	-	7470A	PPB	27 Jul 2020 12:56:54	U	SMPL
CCB72 - 1	CCB72	-80	-0.0630	-	7470A	PPB	27 Jul 2020 12:59:01	U	SMPL
L3383-23 - 1	CRT-015	-3	-0.0396	-	7470A	PPB	27 Jul 2020 13:01:08	U	SMPL
L3383-27 - 1	CRT-014	36	-0.0277	-	7470A	PPB	27 Jul 2020 13:03:14	U	SMPL
L3383-31 - 1	CRT-002	60	-0.0204	-	7470A	PPB	27 Jul 2020 13:05:20	U	SMPL
L3414-04 - 1	61820	73	-0.0165	-	7470A	PPB	27 Jul 2020 13:07:27	U	SMPL
PB130478BL - 1	PBW	74	-0.0162	-	7470A	PPB	27 Jul 2020 13:09:33	U	SMPL
PB130478BS - 1	LCSW	11892	3.5743	-	7470A	PPB	27 Jul 2020 13:11:40	U	SMPL
L3378-17 - 1	DRUM-WATER	-76	-0.0617	-	7470A	PPB	27 Jul 2020 13:13:48	U	SMPL
L3410-04 - 1	FM-FRAC	57	-0.0213	-	7470A	PPB	27 Jul 2020 13:15:55	U	SMPL
L3410-04DUP - 1	FM-FRACDUP	61	-0.0201	-	7470A	PPB	27 Jul 2020 13:18:03	U	SMPL
L3410-04MS - 1	FM-FRACMS	13192	3.9693	-	7470A	PPB	27 Jul 2020 13:20:10	U	SMPL
CCV73 - 1	CCV73	17359	5.2352	-	7470A	PPB	27 Jul 2020 13:22:16	U	SMPL
CCB73 - 1	CCB73	-214	-0.1037	-	7470A	PPB	27 Jul 2020 13:24:22	U	SMPL
L3410-04MSD - 1	FM-FRACMSD	12643	3.8025	-	7470A	PPB	27 Jul 2020 13:26:29	U	SMPL
PB130489BL - 1	PBW	-32	-0.0484	-	7470A	PPB	27 Jul 2020 13:31:15	U	SMPL
PB130489BS - 1	LCSW	13022	3.9176	-	7470A	PPB	27 Jul 2020 13:33:21	U	SMPL
L3405-01 - 1	0437-MODIFIED-ELUTRIATE	107	-0.0061	-	7470A	PPB	27 Jul 2020 13:35:27	U	SMPL
L3405-02 - 1	0437-MODIFIED-ELUTRIATE	172	0.0136	-	7470A	PPB	27 Jul 2020 13:37:34	U	SMPL
L3410-03 - 1	FM-FRAC	1353	0.3724	-	7470A	PPB	27 Jul 2020 13:39:41	U	SMPL
L3410-03DUP - 1	FM-FRACDUP	1484	0.4122	-	7470A	PPB	27 Jul 2020 13:44:26	U	SMPL
L3410-03MS - 1	FM-FRACMS	14854	4.4742	-	7470A	PPB	27 Jul 2020 13:46:33	U	SMPL
L3410-03MSD - 1	FM-FRACMSD	15155	4.5656	-	7470A	PPB	27 Jul 2020 13:48:41	U	SMPL
L3450-02 - 1	TT-016-IDWGW-20200723	1853	0.5243	-	7470A	PPB	27 Jul 2020 13:50:48	U	SMPL
CCV74 - 1	CCV74	12744	3.8331	-	7470A	PPB	27 Jul 2020 13:52:56	U	SMPL
CCB74 - 1	CCB74	0	-0.0387	-	7470A	PPB	27 Jul 2020 13:55:02	U	SMPL
CCV74 - 1	CCV74	16225	4.8907	-	7470A	PPB	27 Jul 2020 13:55:32	U	SMPL
CCB74 - 1	CCB74	-153	-0.0851	-	7470A	PPB	27 Jul 2020 13:57:39	U	SMPL
L3450-03 - 1	TT-017-IDWGW-20200723	1994	0.5671	-	7470A	PPB	27 Jul 2020 13:59:46	U	SMPL
L3450-04 - 1	TT-018-IDWGW-20200723	1761	0.4964	-	7470A	PPB	27 Jul 2020 14:01:52	U	SMPL
L3457-01 - 1	SHB-MOTOR-ROOM	130	0.0008	-	7470A	PPB	27 Jul 2020 14:03:59	U	SMPL
PB130475TB - 1	PB130429TB	59	-0.0207	-	7470A	PPB	27 Jul 2020 14:06:05	U	SMPL
PB130478TB - 1	PB130454TB	103	-0.0074	-	7470A	PPB	27 Jul 2020 14:08:12	U	SMPL
L3382-03LX5 - 1		262	0.0409	-	7470A	PPB	27 Jul 2020 14:10:19	U	SMPL
L3382-03A - 1		13084	3.9364	-	7470A	PPB	27 Jul 2020 14:12:26	U	SMPL
L3410-04LX5 - 1		102	-0.0077	-	7470A	PPB	27 Jul 2020 14:14:34	U	SMPL
L3410-04A - 1		12278	3.6916	-	7470A	PPB	27 Jul 2020 14:16:41	U	SMPL
PB130475BL - 1	PBW	133	0.0017	-	7470A	PPB	27 Jul 2020 14:18:49	U	SMPL
CCV75 - 1	CCV75	16785	5.0609	-	7470A	PPB	27 Jul 2020 14:20:55	U	SMPL
CCB75 - 1	CCB75	-62	-0.0575	-	7470A	PPB	27 Jul 2020 14:23:02	U	SMPL
L3410-03LX5 - 1		382	0.0774	-	7470A	PPB	27 Jul 2020 14:25:11	U	SMPL
L3410-03A - 1		14823	4.4648	-	7470A	PPB	27 Jul 2020 14:27:17	U	SMPL
CCV76 - 1	CCV76	16340	4.9257	-	7470A	PPB	27 Jul 2020 14:29:24	U	SMPL
CCB76 - 1	CCB76	-205	-0.1009	-	7470A	PPB	27 Jul 2020 14:31:33	U	SMPL