


LB110264

ISM02.4

INSTRUMENT ID: CV1

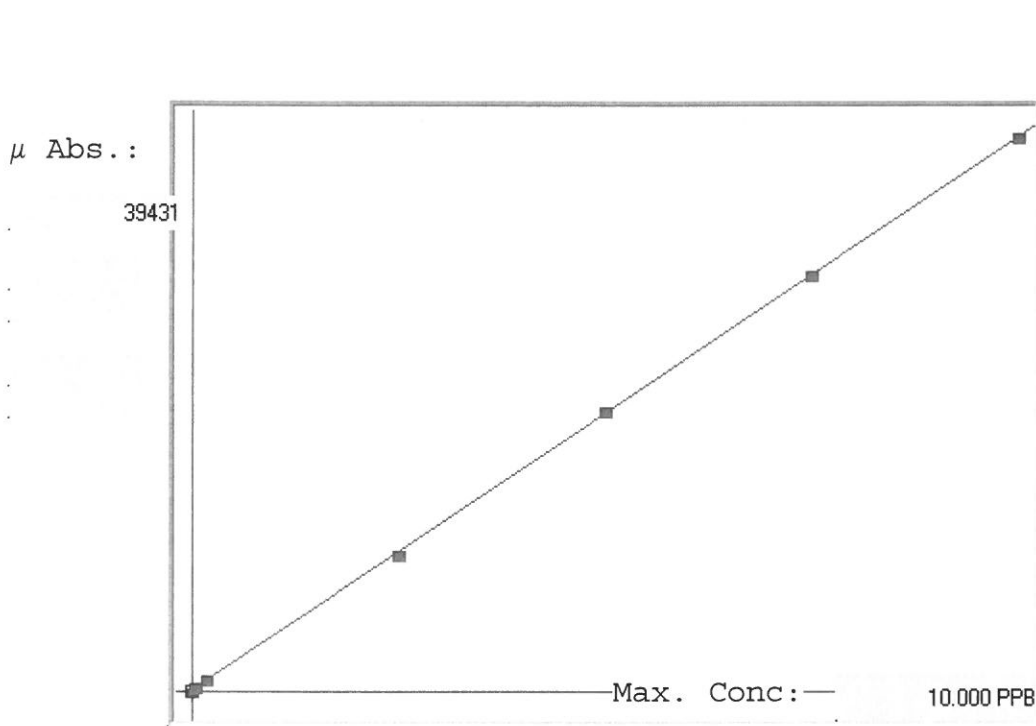

Linear

A= 0.0000e+000

B= 2.5353e-004

C= -1.6547e-002

Rho= 0.9999837

Accept=Accepted

*skype*  
*y=13715xcept*

| Std ID | Conc.  | Calc.  | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | %D |
|--------|--------|--------|--------|-------|------------|-------|-------|-------|-------|-------|----|
| 0.00   | 0.000  | -0.008 | -0.008 | 34    | 0.000      | 34    |       |       |       |       | 16 |
| 0.05   | 0.050  | 0.058  | 0.008  | 294   | 0.0 %      | 294   |       |       |       |       | 2  |
| 0.20   | 0.200  | 0.204  | 0.004  | 870   | 0.0 %      | 870   |       |       |       |       | -1 |
| 2.50   | 2.500  | 2.467  | -0.033 | 9794  | 0.0 %      | 9794  |       |       |       |       | 1  |
| 5.00   | 5.000  | 5.037  | 0.037  | 19932 | 0.0 %      | 19932 |       |       |       |       | 0  |
| 7.50   | 7.500  | 7.512  | 0.012  | 29695 | 0.0 %      | 29695 |       |       |       |       | 0  |
| 10.0   | 10.000 | 9.980  | -0.020 | 39431 | 0.0 %      | 39431 |       |       |       |       | 0  |

LB110264  
INSTRUMENT ID : CV1

| Sample ID  | Extended ID | $\mu$ Abs. | Conc.     | Std Conc | Method    | Units | Date            | Type |
|------------|-------------|------------|-----------|----------|-----------|-------|-----------------|------|
|            | 0 S0.05     | 34         | -         |          | 0 ISM02.4 | PPB   | 7/29/2020 10:46 | Std  |
|            | 0.05 S0.05  | 294        | -         | 0.05     | ISM02.4   | PPB   | 7/29/2020 10:48 | Std  |
|            | 0.2 S0.2    | 870        | -         | 0.2      | ISM02.4   | PPB   | 7/29/2020 10:51 | Std  |
|            | 2.5 S2.5    | 9794       | -         | 2.5      | ISM02.4   | PPB   | 7/29/2020 10:53 | Std  |
|            | 5 S5.0      | 19932      | -         | 5        | ISM02.4   | PPB   | 7/29/2020 11:02 | Std  |
|            | 7.5 S7.5    | 29695      | -         | 7.5      | ISM02.4   | PPB   | 7/29/2020 11:05 | Std  |
|            | 10 S10.0    | 39431      | -         | 10       | ISM02.4   | PPB   | 7/29/2020 11:12 | Std  |
| ICV        | ICV         | 15716      | 3.968 -   |          | ISM02.4   | PPB   | 7/29/2020 11:18 | SMPL |
| ICB        | ICB         | 116        | 0.0129 -  |          | ISM02.4   | PPB   | 7/29/2020 11:27 | SMPL |
| CCV001     | CCV001      | 19928      | 5.0358 -  |          | ISM02.4   | PPB   | 7/29/2020 11:29 | SMPL |
| CCB001     | CCB001      | 31         | -0.0087 - |          | ISM02.4   | PPB   | 7/29/2020 11:37 | SMPL |
| PB130560BL | PBW560      | -15        | -0.0203 - |          | ISM02.4   | PPB   | 7/29/2020 11:39 | SMPL |
| L3447-01   | MBFS50      | 2290       | 0.564 -   |          | ISM02.4   | PPB   | 7/29/2020 11:41 | SMPL |
| L3447-02   | MBFS56      | 3705       | 0.9228 -  |          | ISM02.4   | PPB   | 7/29/2020 11:53 | SMPL |
| L3447-03   | MBFS56D     | 3883       | 0.9679 -  |          | ISM02.4   | PPB   | 7/29/2020 12:00 | SMPL |
| L3447-04   | MBFS56S     | 7982       | 2.0071 -  |          | ISM02.4   | PPB   | 7/29/2020 12:03 | SMPL |
| PB130561BL | PBW561      | 120        | 0.0139 -  |          | ISM02.4   | PPB   | 7/29/2020 12:05 | SMPL |
| L3448-01   | MBFS51      | 16         | -0.0125 - |          | ISM02.4   | PPB   | 7/29/2020 12:07 | SMPL |
| L3448-02   | MBFS57      | 857        | 0.2007 -  |          | ISM02.4   | PPB   | 7/29/2020 12:14 | SMPL |
| L3448-03   | MBFS57D     | 876        | 0.2055 -  |          | ISM02.4   | PPB   | 7/29/2020 12:17 | SMPL |
| L3448-04   | MBFS57S     | 4314       | 1.0772 -  |          | ISM02.4   | PPB   | 7/29/2020 12:22 | SMPL |
| CCV002     | CCV002      | 18921      | 4.7805 -  |          | ISM02.4   | PPB   | 7/29/2020 12:24 | SMPL |
| CCB002     | CCB002      | -30        | -0.0242 - |          | ISM02.4   | PPB   | 7/29/2020 12:26 | SMPL |