


LB110342

245.1

INSTRUMENT ID: CV1

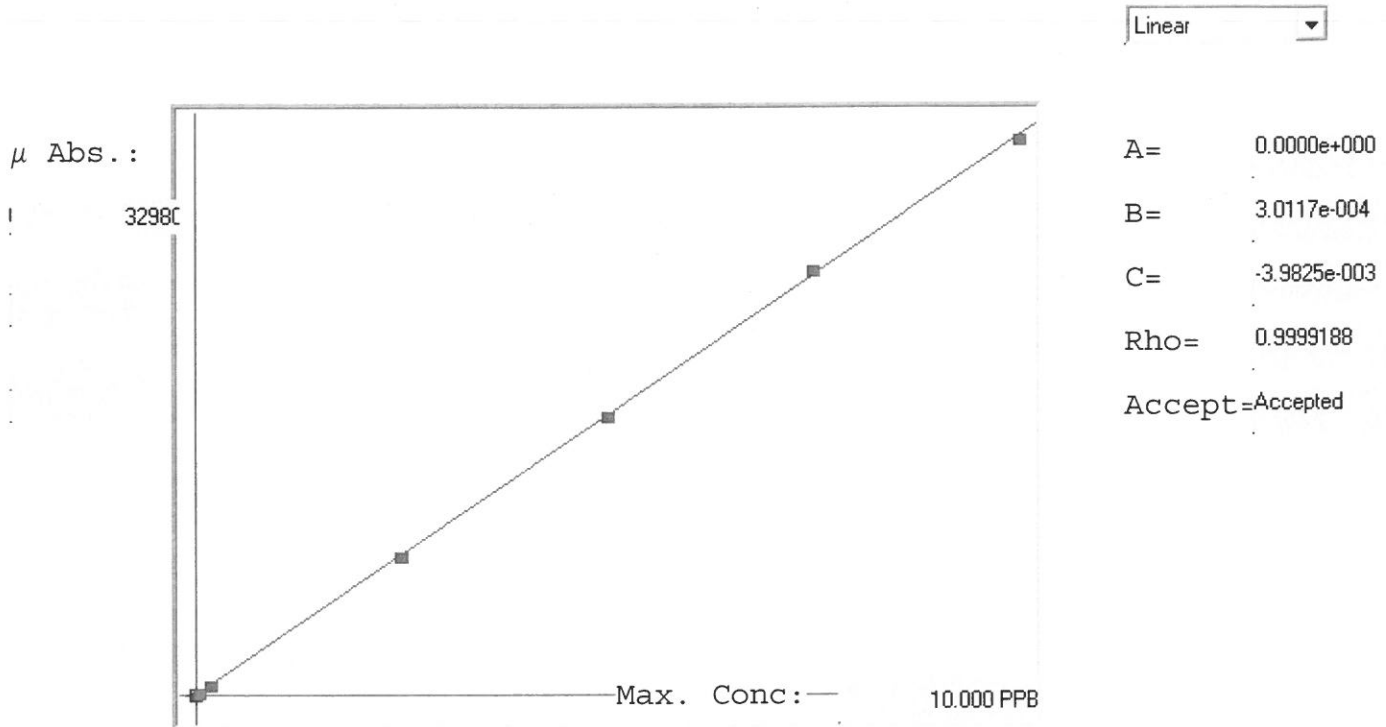

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.002	0.002	19	0.000	19				
0.05	0.050	0.049	-0.001	175	0.0 %	175				
0.2	0.200	0.187	-0.013	634	0.0 %	634				
2.5	2.500	2.489	-0.011	8277	0.0 %	8277				
5.0	5.000	4.994	-0.006	16595	0.0 %	16595				
7.5	7.500	7.601	0.101	25252	0.0 %	25252				
10.0	10.000	9.929	-0.071	32980	0.0 %	32980				

LB110342 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 03 Aug 2020 16:11:51

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	19	-	0.0000	245.1	PPB	03 Aug 2020 16:16:41	S	Std
0.05 - 1	50.05	175	-	0.0500	245.1	PPB	03 Aug 2020 16:18:59	S	Std
0.2 - 1	50.2	634	-	0.2000	245.1	PPB	03 Aug 2020 16:21:16	S	Std
2.5 - 1	52.5	8277	-	2.5000	245.1	PPB	03 Aug 2020 16:23:33	S	Std
5.0 - 1	55	16595	-	5.0000	245.1	PPB	03 Aug 2020 16:25:49	S	Std
7.5 - 1	57.5	25252	-	7.5000	245.1	PPB	03 Aug 2020 16:28:05	S	Std
10.0 - 1	510	32980	-	10.0000	245.1	PPB	03 Aug 2020 16:32:59	S	Std
ICV53 - 1	ICV53	12822	3.8576	-245.1		PPB	03 Aug 2020 16:40:52	U	SMPL
ICB53 - 1	ICB53	-49	-0.0187	-245.1		PPB	03 Aug 2020 16:45:43	U	SMPL
CCV42 - 1	CCV42	17223	5.1831	-245.1		PPB	03 Aug 2020 16:47:57	U	SMPL
CCB42 - 1	CCB42	-46	-0.0178	-245.1		PPB	03 Aug 2020 16:52:47	U	SMPL
CRA - 1	CRA	151	0.0415	-245.1		PPB	03 Aug 2020 16:57:32	U	SMPL
HighStd - 1	HighStd	33349	10.0398	-245.1		PPB	03 Aug 2020 16:59:47	U	SMPL
ChkStd - 1	ChkStd	24153	7.2702	-245.1		PPB	03 Aug 2020 17:02:03	U	SMPL
PB130716BL - 1	PBW	-26	-0.0118	-245.1		PPB	03 Aug 2020 17:06:55	U	SMPL
PB130716BS - 1	LCSW	13141	3.9537	-245.1		PPB	03 Aug 2020 17:09:11	U	SMPL
L3319-05 - 1	PT-HG-WS	8161	2.4539	-245.1		PPB	03 Aug 2020 17:18:18	U	SMPL
CCV43 - 1	CCV43	17046	5.1298	-245.1		PPB	03 Aug 2020 17:25:21	U	SMPL
CCB43 - 1	CCB43	-70	-0.0251	-245.1		PPB	03 Aug 2020 17:30:05	U	SMPL