


LB110436

245.1

INSTRUMENT ID: CV1

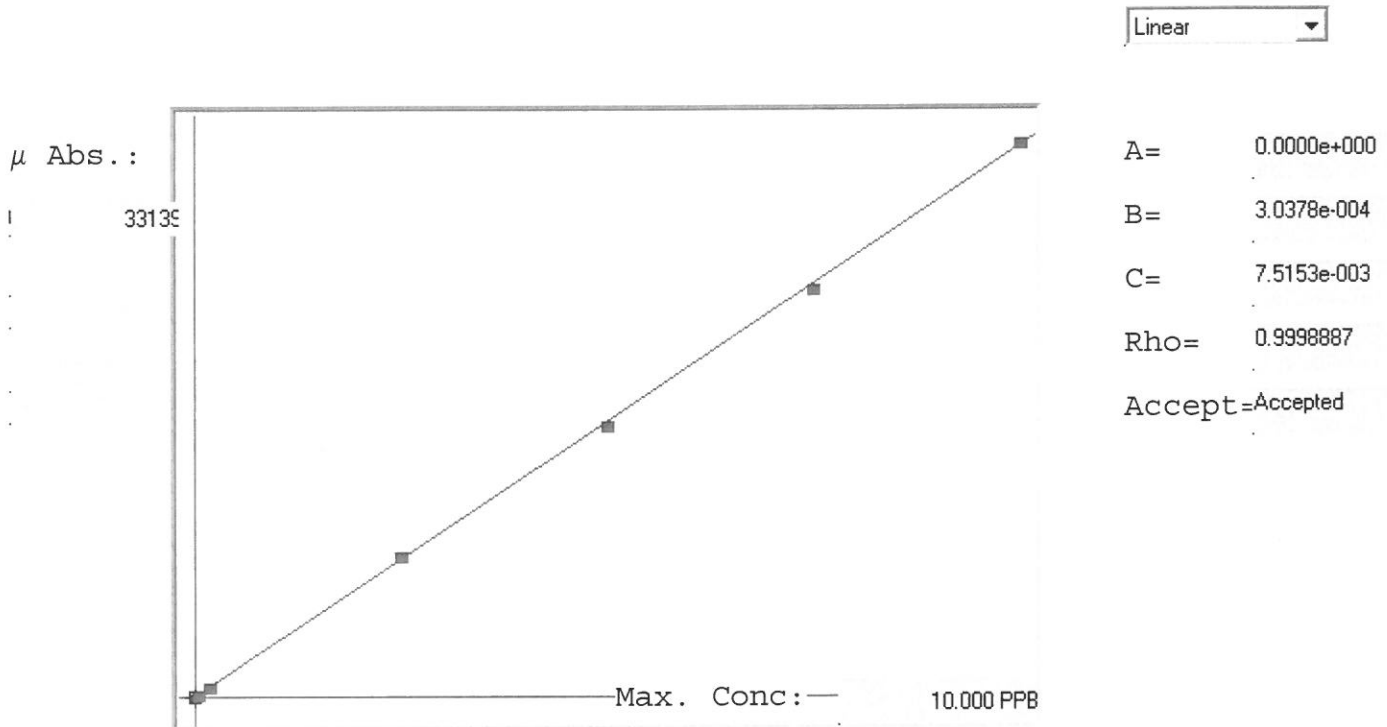

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.002	0.002	-19	0.000	-19				
0.05	0.050	0.058	0.008	167	0.0 %	167				
0.2	0.200	0.190	-0.010	602	0.0 %	602				
2.5	2.500	2.570	0.070	8434	0.0 %	8434				
5.0	5.000	4.942	-0.058	16244	0.0 %	16244				
7.5	7.500	7.413	-0.087	24378	0.0 %	24378				
10.0	10.000	10.075	0.075	33139	0.0 %	33139				

LB110436 INSTRUMENT ID : CV1

Method: 245.1		Operator: Admin		Date of Analysis: 07 Aug 2020 17:33:13				
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	58	-19	-	0.0000245.1	PPB	07 Aug 2020 18:16:10	S	Std
0.05 - 1	58.05	167	-	0.0500245.1	PPB	07 Aug 2020 18:18:27	S	Std
0.2 - 1	58.2	602	-	0.2000245.1	PPB	07 Aug 2020 18:20:44	S	Std
2.5 - 1	52.5	8434	-	2.5000245.1	PPB	07 Aug 2020 18:23:02	S	Std
5.0 - 1	55	16244	-	5.0000245.1	PPB	07 Aug 2020 18:25:18	S	Std
7.5 - 1	57.5	24378	-	7.5000245.1	PPB	07 Aug 2020 18:27:34	S	Std
10.0 - 1	510	33139	-	10.0000245.1	PPB	07 Aug 2020 18:32:28	S	Std
ICV60 - 1	ICV60	12635	3.8458	-245.1	PPB	07 Aug 2020 18:37:50	U	SMPL
ICB60 - 1	ICB60	4	0.0087	-245.1	PPB	07 Aug 2020 18:42:37	U	SMPL
CCV76 - 1	CCV76	16423	4.9966	-245.1	PPB	07 Aug 2020 18:44:52	U	SMPL
CCB76 - 1	CCB76	-1	0.0072	-245.1	PPB	07 Aug 2020 18:49:39	U	SMPL
CRA - 1	CRA	155	0.0546	-245.1	PPB	07 Aug 2020 18:51:54	U	SMPL
HighStd - 1	HighStd	33008	10.0348	-245.1	PPB	07 Aug 2020 18:54:08	U	SMPL
ChkStd - 1	ChkStd	23867	7.2579	-245.1	PPB	07 Aug 2020 18:56:24	U	SMPL
PB130830BL - 1	PBW	-14	0.0033	-245.1	PPB	07 Aug 2020 19:01:16	U	SMPL
PB130830BS - 1	LCSW	12702	3.8662	-245.1	PPB	07 Aug 2020 19:03:31	U	SMPL
L3216-12 - 1	MDL-WATER-06-QT3-2020	151	0.0534	-245.1	PPB	07 Aug 2020 19:08:20	U	SMPL
L3569-02 - 1	COMP	297	0.0977	-245.1	PPB	07 Aug 2020 19:15:26	U	SMPL
L3569-02DUP - 1	COMPDUP	225	0.0759	-245.1	PPB	07 Aug 2020 19:17:43	U	SMPL
L3569-02MS - 1	COMPMS	12420	3.7805	-245.1	PPB	07 Aug 2020 19:22:30	U	SMPL
L3569-02MSD - 1	COMPMSD	13985	4.2559	-245.1	PPB	07 Aug 2020 19:24:45	U	SMPL
CCV77 - 1	CCV77	16236	4.9398	-245.1	PPB	07 Aug 2020 19:27:00	U	SMPL
CCB77 - 1	CCB77	18	0.0130	-245.1	PPB	07 Aug 2020 19:31:48	U	SMPL
L3605-01 - 1	DW-QUAL-HOGHOUSE	-10	0.0045	-245.1	PPB	07 Aug 2020 19:34:03	U	SMPL
L3569-02LX5 - 1		125	0.0455	-245.1	PPB	07 Aug 2020 19:36:18	U	SMPL
L3569-02A - 1		14152	4.3067	-245.1	PPB	07 Aug 2020 19:38:34	U	SMPL
CCV78 - 1	CCV78	16165	4.9182	-245.1	PPB	07 Aug 2020 19:40:50	U	SMPL
CCB78 - 1	CCB78	0	0.0075	-245.1	PPB	07 Aug 2020 19:45:36	U	SMPL