

LB11046T


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

30868

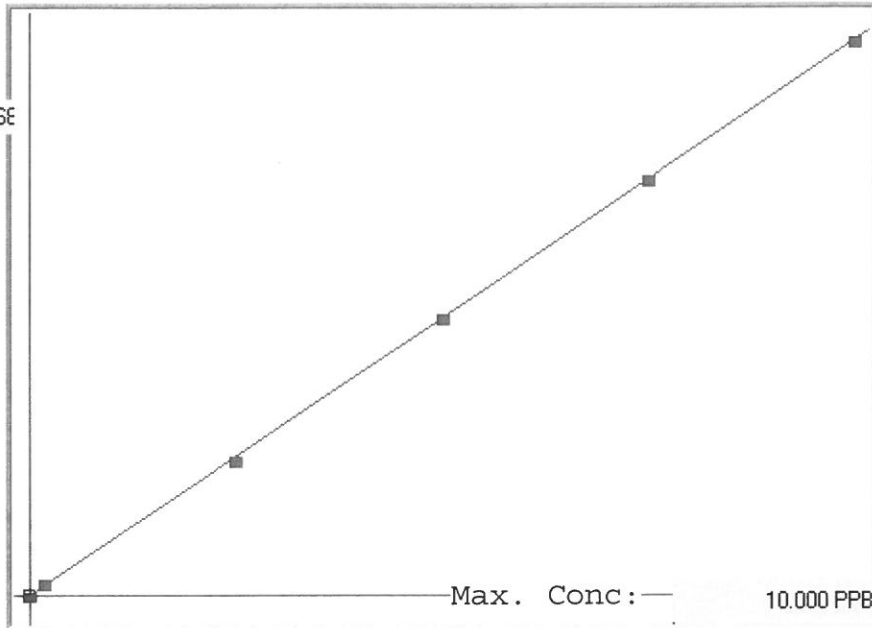

A= 0.0000e+000

B= 3.2354e-004

C= 9.7037e-003

Rho= 0.9999712

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.005	0.005	-15	0.000	-15				
0.2	0.200	0.227	0.027	671	0.0 %	671				
2.5	2.500	2.442	-0.058	7517	0.0 %	7517				
5.0	5.000	5.022	0.022	15493	0.0 %	15493				
7.5	7.500	7.508	0.008	23175	0.0 %	23175				
10.0	10.000	9.997	-0.003	30868	0.0 %	30868				

LB110465 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 11 Aug 2020 08:40:22					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-15	-	0.0007	7470A	PPB	11 Aug 2020 08:55:15	S	Std
0.2 - 1	50.2	671	-	0.2007	7470A	PPB	11 Aug 2020 09:00:42	S	Std
2.5 - 1	52.5	7517	-	2.5007	7470A	PPB	11 Aug 2020 09:02:51	S	Std
5.0 - 1	55	15493	-	5.0007	7470A	PPB	11 Aug 2020 09:04:58	S	Std
7.5 - 1	57.5	23175	-	7.5007	7470A	PPB	11 Aug 2020 09:07:05	S	Std
10.0 - 1	510	30868	-	10.0007	7470A	PPB	11 Aug 2020 09:11:36	S	Std
ICV62 - 1	ICV62	12000	3.8922	-	7470A	PPB	11 Aug 2020 09:14:05	U	SMPL
ICB62 - 1	ICB62	-166	-0.0440	-	7470A	PPB	11 Aug 2020 09:16:12	U	SMPL
CCV88 - 1	CCV88	16213	5.2552	-	7470A	PPB	11 Aug 2020 09:18:19	U	SMPL
CCB88 - 1	CCB88	-160	-0.0421	-	7470A	PPB	11 Aug 2020 09:20:25	U	SMPL
CRA - 1	CRA	670	0.2265	-	7470A	PPB	11 Aug 2020 09:22:32	U	SMPL
HighStd - 1	HighStd	30905	10.0086	-	7470A	PPB	11 Aug 2020 09:24:38	U	SMPL
ChkStd - 1	ChkStd	22700	7.3540	-	7470A	PPB	11 Aug 2020 09:26:44	U	SMPL
PB130860BL - 1	PBW	-332	-0.0977	-	7470A	PPB	11 Aug 2020 09:28:53	U	SMPL
PB130860BS - 1	LCSW	10258	3.3286	-	7470A	PPB	11 Aug 2020 09:31:01	U	SMPL
L3478-05 - 1	ROLLOFF-VNJ-213	-177	-0.0476	-	7470A	PPB	11 Aug 2020 09:33:08	U	SMPL
L3506-05 - 1	OR-02-080720	-39	-0.0029	-	7470A	PPB	11 Aug 2020 09:35:16	U	SMPL
L3506-05DUP - 1	OR-02-080720DUP	16	0.0149	-	7470A	PPB	11 Aug 2020 09:37:24	U	SMPL
L3506-05MS - 1	OR-02-080720MS	12136	3.9362	-	7470A	PPB	11 Aug 2020 09:39:32	U	SMPL
L3506-05MSD - 1	OR-02-080720MSD	10783	3.4984	-	7470A	PPB	11 Aug 2020 09:41:38	U	SMPL
CCV89 - 1	CCV89	16778	5.4380	-	7470A	PPB	11 Aug 2020 09:43:45	U	SMPL
CCB89 - 1	CCB89	-164	-0.0434	-	7470A	PPB	11 Aug 2020 09:45:51	U	SMPL
PB130861BL - 1	PBW	-29	0.0003	-	7470A	PPB	11 Aug 2020 09:52:33	U	SMPL
PB130861BS - 1	LCSW	11136	3.6126	-	7470A	PPB	11 Aug 2020 09:54:39	U	SMPL
L3607-02 - 1	ES-TOTE-COMP	-154	-0.0401	-	7470A	PPB	11 Aug 2020 09:56:45	U	SMPL
L3607-02DUP - 1	ES-TOTE-COMPDUP	-16	0.0045	-	7470A	PPB	11 Aug 2020 09:58:52	U	SMPL
L3607-02MS - 1	ES-TOTE-COMPMS	11472	3.7213	-	7470A	PPB	11 Aug 2020 10:00:59	U	SMPL
L3607-02MSD - 1	ES-TOTE-COMPMSD	11208	3.6359	-	7470A	PPB	11 Aug 2020 10:03:06	U	SMPL
PB130862BL - 1	PBW	-181	-0.0489	-	7470A	PPB	11 Aug 2020 10:05:15	U	SMPL
PB130862BS - 1	LCSW	11671	3.7857	-	7470A	PPB	11 Aug 2020 10:07:23	U	SMPL
L3607-01 - 1	ES-TOTE-COMP	348	0.1223	-	7470A	PPB	11 Aug 2020 10:09:30	U	SMPL
CCV90 - 1	CCV90	16372	5.3067	-	7470A	PPB	11 Aug 2020 10:11:37	U	SMPL
CCB90 - 1	CCB90	-161	-0.0424	-	7470A	PPB	11 Aug 2020 10:13:43	U	SMPL
L3607-01DUP - 1	ES-TOTE-COMPDUP	220	0.0809	-	7470A	PPB	11 Aug 2020 10:21:04	U	SMPL
L3607-01MS - 1	ES-TOTE-COMPMS	14437	4.6806	-	7470A	PPB	11 Aug 2020 10:23:10	U	SMPL
L3607-01MSD - 1	ES-TOTE-COMPMSD	13864	4.4952	-	7470A	PPB	11 Aug 2020 10:25:16	U	SMPL
L3614-01 - 1	0495-MODIFIED-ELUTRIATE	216	0.0796	-	7470A	PPB	11 Aug 2020 10:27:24	U	SMPL
L3614-02 - 1	0495-MODIFIED-ELUTRIATE	216	0.0796	-	7470A	PPB	11 Aug 2020 10:29:31	U	SMPL
PB130866BL - 1	PBW	-42	-0.0039	-	7470A	PPB	11 Aug 2020 10:36:15	U	SMPL
PB130866BS - 1	LCSW	11015	3.5735	-	7470A	PPB	11 Aug 2020 10:38:22	U	SMPL
L3626-01 - 1	1717	284	0.1016	-	7470A	PPB	11 Aug 2020 10:40:29	U	SMPL
L3626-01DUP - 1	1717DUP	356	0.1249	-	7470A	PPB	11 Aug 2020 10:42:38	U	SMPL
L3626-01MS - 1	1717MS	12832	4.1613	-	7470A	PPB	11 Aug 2020 10:44:44	U	SMPL
CCV91 - 1	CCV91	13988	4.5353	-	7470A	PPB	11 Aug 2020 10:46:50	U	SMPL
CCB91 - 1	CCB91	-110	-0.0259	-	7470A	PPB	11 Aug 2020 10:48:57	U	SMPL
L3626-01MSD - 1	1717MSD	12951	4.1998	-	7470A	PPB	11 Aug 2020 10:51:05	U	SMPL
PB130860TB - 1	PB130826TB	-170	-0.0453	-	7470A	PPB	11 Aug 2020 10:53:11	U	SMPL
PB130861TB - 1	PB130828TB	-11	0.0061	-	7470A	PPB	11 Aug 2020 10:55:19	U	SMPL
PB130866TB - 1	PB130863TB	65	0.0307	-	7470A	PPB	11 Aug 2020 10:57:26	U	SMPL
CCV92 - 1	CCV92	16139	5.2313	-	7470A	PPB	11 Aug 2020 10:59:33	U	SMPL
CCB92 - 1	CCB92	-125	-0.0307	-	7470A	PPB	11 Aug 2020 11:01:39	U	SMPL
L3506-05LX5 - 1		58	0.0285	-	7470A	PPB	11 Aug 2020 11:03:47	U	SMPL
L3506-05A - 1		10412	3.3784	-	7470A	PPB	11 Aug 2020 11:05:55	U	SMPL
L3607-02LX5 - 1		-85	-0.0178	-	7470A	PPB	11 Aug 2020 11:08:03	U	SMPL
L3607-02A - 1		10860	3.5233	-	7470A	PPB	11 Aug 2020 11:10:12	U	SMPL
L3607-01LX5 - 1		-57	-0.0087	-	7470A	PPB	11 Aug 2020 11:12:18	U	SMPL
L3607-01A - 1		13992	4.5366	-	7470A	PPB	11 Aug 2020 11:14:26	U	SMPL
L3626-01LX5 - 1		-49	-0.0061	-	7470A	PPB	11 Aug 2020 11:16:32	U	SMPL
L3626-01A - 1		12691	4.1157	-	7470A	PPB	11 Aug 2020 11:18:40	U	SMPL
CCV93 - 1	CCV93	15156	4.9132	-	7470A	PPB	11 Aug 2020 11:20:46	U	SMPL
CCB93 - 1	CCB93	-123	-0.0301	-	7470A	PPB	11 Aug 2020 11:22:53	U	SMPL