


LB 110635

7470A

INSTRUMENT ID: CV4

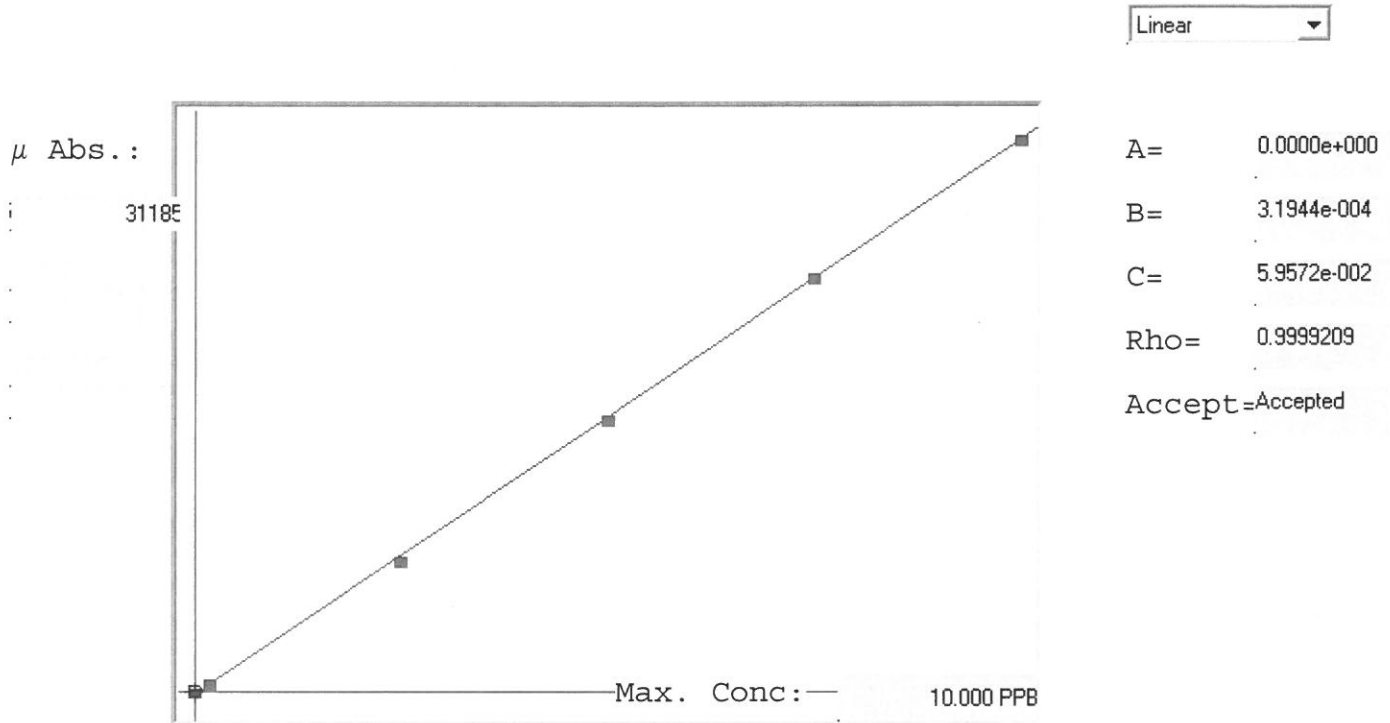

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.058	0.058	-5	0.000	-5				
0.2	0.200	0.218	0.018	495	0.0 %	495				
2.5	2.500	2.408	-0.092	7352	0.0 %	7352				
5.0	5.000	4.985	-0.015	15418	0.0 %	15418				
7.5	7.500	7.510	0.010	23325	0.0 %	23325				
10.0	10.000	10.021	0.021	31185	0.0 %	31185				

LB110635 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 21 Aug 2020 08:53:57

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-5	-	0.0000	7470A	PPB	21 Aug 2020 08:57:38	S	Std
0.2 - 1	50.2	495	-	0.2000	7470A	PPB	21 Aug 2020 08:59:46	S	Std
2.5 - 1	52.5	7352	-	2.5000	7470A	PPB	21 Aug 2020 09:01:53	S	Std
5.0 - 1	55	15418	-	5.0000	7470A	PPB	21 Aug 2020 09:04:01	S	Std
7.5 - 1	57.5	23325	-	7.5000	7470A	PPB	21 Aug 2020 09:08:32	S	Std
10.0 - 1	510	31185	-	10.0000	7470A	PPB	21 Aug 2020 09:10:38	S	Std
ICV77 - 1	ICV77	12998	4.2116	-7470A	PPB	21 Aug 2020 09:13:12	U	SMPL	
ICB77 - 1	ICB77	-271	-0.0270	-7470A	PPB	21 Aug 2020 09:15:18	U	SMPL	
CCV59 - 1	CCV59	16277	5.2590	-7470A	PPB	21 Aug 2020 09:17:24	U	SMPL	
CCB59 - 1	CCB59	-273	-0.0276	-7470A	PPB	21 Aug 2020 09:19:30	U	SMPL	
CRA - 1	CRA	435	0.1985	-7470A	PPB	21 Aug 2020 09:21:37	U	SMPL	
HighStd - 1	HighStd	31188	10.0222	-7470A	PPB	21 Aug 2020 09:23:43	U	SMPL	
ChkStd - 1	ChkStd	23307	7.5047	-7470A	PPB	21 Aug 2020 09:25:49	U	SMPL	
PB131119BL - 1	PBW	-367	-0.0577	-7470A	PPB	21 Aug 2020 09:27:58	U	SMPL	
PB131119BS - 1	LCSW	11525	3.7411	-7470A	PPB	21 Aug 2020 09:30:06	U	SMPL	
L3502-15 - 1	OK-02-081920	-226	-0.0126	-7470A	PPB	21 Aug 2020 09:32:13	U	SMPL	
L3502-15DUP - 1	OK-02-081920DUP	-100	0.0276	-7470A	PPB	21 Aug 2020 09:34:21	U	SMPL	
L3502-15MS - 1	OK-02-081920MS	12551	4.0688	-7470A	PPB	21 Aug 2020 09:36:29	U	SMPL	
L3502-15MSD - 1	OK-02-081920MSD	12209	3.9596	-7470A	PPB	21 Aug 2020 09:38:37	U	SMPL	
L3504-12 - 1	EO-01-081920	-252	-0.0209	-7470A	PPB	21 Aug 2020 09:40:43	U	SMPL	
CCV60 - 1	CCV60	16169	5.2245	-7470A	PPB	21 Aug 2020 09:42:50	U	SMPL	
CCB60 - 1	CCB60	-285	-0.0315	-7470A	PPB	21 Aug 2020 09:44:56	U	SMPL	
L3731-01 - 1	POLY-DRUM	145	0.1059	-7470A	PPB	21 Aug 2020 09:47:03	U	SMPL	
L3742-04 - 1	TP-10-S	-61	0.0401	-7470A	PPB	21 Aug 2020 09:49:08	U	SMPL	
L3742-08 - 1	TP-10-D	-37	0.0478	-7470A	PPB	21 Aug 2020 09:51:14	U	SMPL	
PB131119TB - 1	PB131101TB	-26	0.0513	-7470A	PPB	21 Aug 2020 09:53:21	U	SMPL	
L3502-15LX5 - 1		-28	0.0506	-7470A	PPB	21 Aug 2020 09:55:27	U	SMPL	
L3502-15A - 1		12326	3.9969	-7470A	PPB	21 Aug 2020 09:57:34	U	SMPL	
CCV61 - 1	CCV61	16043	5.1843	-7470A	PPB	21 Aug 2020 09:59:42	U	SMPL	
CCB61 - 1	CCB61	-250	-0.0203	-7470A	PPB	21 Aug 2020 10:01:50	U	SMPL	