


LB 110 744

7470A

INSTRUMENT ID: CY1

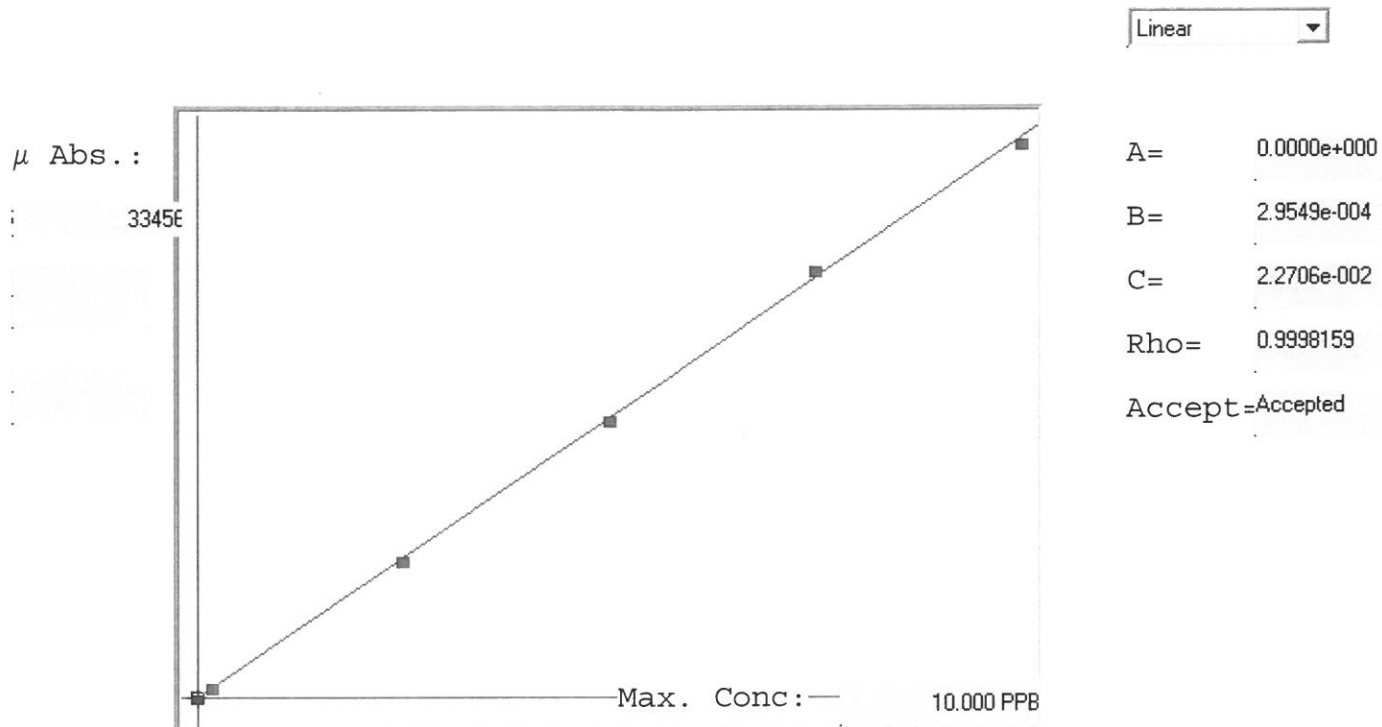

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.011	0.011	-39	0.000	-39				
0.2	0.200	0.194	-0.006	581	0.0 %	581				
2.5	2.500	2.458	-0.042	8240	0.0 %	8240				
5.0	5.000	4.988	-0.012	16805	0.0 %	16805				
7.5	7.500	7.640	0.140	25779	0.0 %	25779				
10.0	10.000	9.909	-0.091	33456	0.0 %	33456				

LB110744 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 31 Aug 2020 09:27:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-39	-	0.0000	7470A	PPB	31 Aug 2020 09:33:50	S	Std
0.2 - 1	50.2	581	-	0.2000	7470A	PPB	31 Aug 2020 09:36:07	S	Std
2.5 - 1	52.5	8240	-	2.5000	7470A	PPB	31 Aug 2020 09:38:25	S	Std
5.0 - 1	55	16805	-	5.0000	7470A	PPB	31 Aug 2020 09:40:41	S	Std
7.5 - 1	57.5	25779	-	7.5000	7470A	PPB	31 Aug 2020 09:45:44	S	Std
10.0 - 1	SV	33456	-	10.0000	7470A	PPB	31 Aug 2020 09:47:59	S	Std
ICV90 - 1	ICV90	13183	3.9181	-7470A	PPB	31 Aug 2020 09:50:40	U	SMPL	
ICB90 - 1	ICB90	-296	-0.0648	-7470A	PPB	31 Aug 2020 09:52:55	U	SMPL	
CCV06 - 1	CCV06	17366	5.1541	-7470A	PPB	31 Aug 2020 09:55:10	U	SMPL	
CCB06 - 1	CCB06	-254	-0.0523	-7470A	PPB	31 Aug 2020 09:57:25	U	SMPL	
CRA - 1	CRA	551	0.1855	-7470A	PPB	31 Aug 2020 09:59:42	U	SMPL	
HighStd - 1	HighStd	33530	9.9304	-7470A	PPB	31 Aug 2020 10:01:56	U	SMPL	
ChkStd - 1	ChkStd	23452	6.9525	-7470A	PPB	31 Aug 2020 10:04:12	U	SMPL	
PB131275BL - 1	PBW	-343	-0.0786	-7470A	PPB	31 Aug 2020 10:06:30	U	SMPL	
PB131275BS - 1	LCSW	13566	4.0313	-7470A	PPB	31 Aug 2020 10:08:48	U	SMPL	
L3507-17 - 1	SU-03-082720	-212	-0.0399	-7470A	PPB	31 Aug 2020 10:11:04	U	SMPL	
L3507-17DUP - 1	SU-03-082720DUP	-86	-0.0027	-7470A	PPB	31 Aug 2020 10:13:22	U	SMPL	
L3507-17MS - 1	SU-03-082720MS	13323	3.9595	-7470A	PPB	31 Aug 2020 10:15:39	U	SMPL	
L3507-17MSD - 1	SU-03-082720MSD	13481	4.0062	-7470A	PPB	31 Aug 2020 10:17:56	U	SMPL	
PB131276BL - 1	PBW	-234	-0.0464	-7470A	PPB	31 Aug 2020 10:20:12	U	SMPL	
CCV07 - 1	CCV07	17644	5.2363	-7470A	PPB	31 Aug 2020 10:22:27	U	SMPL	
CCB07 - 1	CCB07	-243	-0.0491	-7470A	PPB	31 Aug 2020 10:24:43	U	SMPL	
PB131276BS - 1	LCSW	13386	3.9781	-7470A	PPB	31 Aug 2020 10:26:58	U	SMPL	
L3814-11 - 1	08-09-12	255	0.0981	-7470A	PPB	31 Aug 2020 10:43:22	U	SMPL	
L3814-11DUP - 1	08-09-12DUP	90	0.0493	-7470A	PPB	31 Aug 2020 10:45:36	U	SMPL	
L3814-11MS - 1	08-09-12MS	10012	2.9811	-7470A	PPB	31 Aug 2020 10:47:52	U	SMPL	
L3814-11MSD - 1	08-09-12MSD	9681	2.8833	-7470A	PPB	31 Aug 2020 10:50:08	U	SMPL	
L3814-19 - 1	87-88-89-07-10	-133	-0.0166	-7470A	PPB	31 Aug 2020 10:52:25	U	SMPL	
PB131275TB - 1	PB131248TB	-43	0.0100	-7470A	PPB	31 Aug 2020 10:54:43	U	SMPL	
PB131276TB - 1	PB131272TB	-29	0.0141	-7470A	PPB	31 Aug 2020 10:57:00	U	SMPL	
CCV08 - 1	CCV08	17513	5.1976	-7470A	PPB	31 Aug 2020 10:59:18	U	SMPL	
CCB08 - 1	CCB08	-123	-0.0136	-7470A	PPB	31 Aug 2020 11:01:34	U	SMPL	
L3507-17LX5 - 1		-38	0.0115	-7470A	PPB	31 Aug 2020 11:03:49	U	SMPL	
L3507-17A - 1		14154	4.2050	-7470A	PPB	31 Aug 2020 11:06:05	U	SMPL	
L3814-11LX5 - 1		15	0.0271	-7470A	PPB	31 Aug 2020 11:08:20	U	SMPL	
L3814-11A - 1		13252	3.9385	-7470A	PPB	31 Aug 2020 11:10:36	U	SMPL	
CCV09 - 1	CCV09	17077	5.0687	-7470A	PPB	31 Aug 2020 11:12:51	U	SMPL	
CCB09 - 1	CCB09	-211	-0.0396	-7470A	PPB	31 Aug 2020 11:15:07	U	SMPL	