


LB110783

7470A

INSTRUMENT ID: CV2

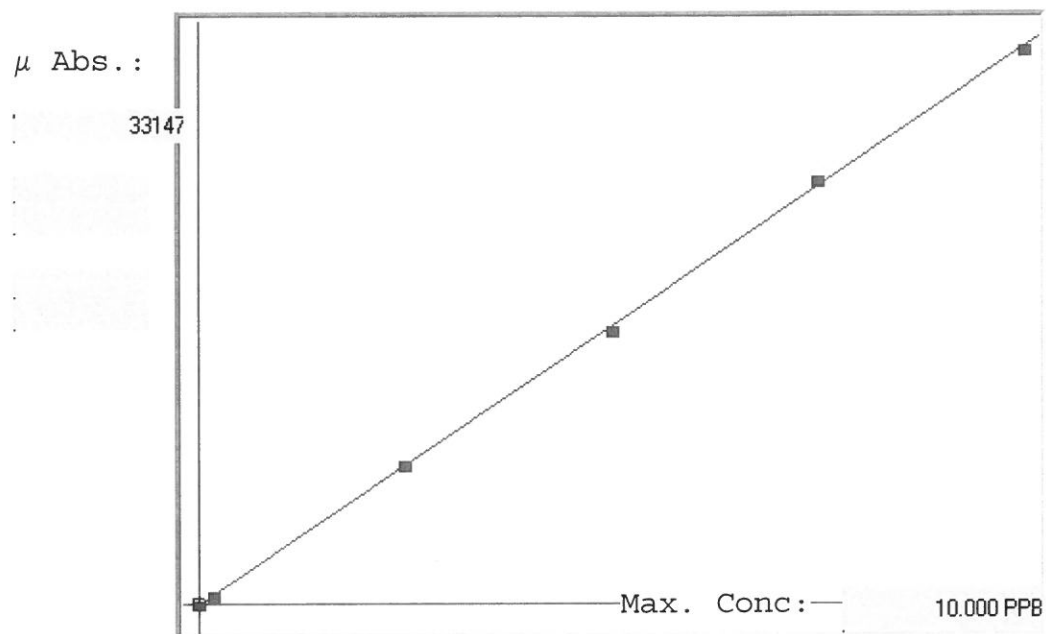

Linear

A= 0.0000e+000

B= 2.9902e-004

C= 3.1049e-002

Rho= 0.9998668

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.003	0.003	-94	0.000	-94				
0.2	0.200	0.196	-0.004	553	0.0 %	553				
2.5	2.500	2.511	0.011	8295	0.0 %	8295				
5.0	5.000	4.930	-0.070	16384	0.0 %	16384				
7.5	7.500	7.616	0.116	25366	0.0 %	25366				
10.0	10.000	9.943	-0.057	33147	0.0 %	33147				

LB110783 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 02 Sep 2020 10:53:26					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-94	-	0.0000	7470A	PPB	02 Sep 2020 11:01:52	S	Std
0.2 - 1	50.2	553	-	0.2000	7470A	PPB	02 Sep 2020 11:04:11	S	Std
2.5 - 1	52.5	8295	-	2.5000	7470A	PPB	02 Sep 2020 11:06:29	S	Std
5.0 - 1	55	16384	-	5.0000	7470A	PPB	02 Sep 2020 11:08:46	S	Std
7.5 - 1	57.5	25366	-	7.5000	7470A	PPB	02 Sep 2020 11:11:02	S	Std
10.0 - 1	50	33147	-	10.0000	7470A	PPB	02 Sep 2020 11:13:18	S	Std
ICV94 - 1	ICV94	13124	3.9554	-	7470A	PPB	02 Sep 2020 11:16:12	U	SMPL
ICB94 - 1	ICB94	-32	0.0215	-	7470A	PPB	02 Sep 2020 11:20:59	U	SMPL
CCV29 - 1	CCV29	17295	5.2027	-	7470A	PPB	02 Sep 2020 11:23:14	U	SMPL
CCB29 - 1	CCB29	-191	-0.0261	-	7470A	PPB	02 Sep 2020 11:25:29	U	SMPL
CRA - 1	CRA	529	0.1892	-	7470A	PPB	02 Sep 2020 11:27:45	U	SMPL
HighStd - 1	HighStd	33567	10.0684	-	7470A	PPB	02 Sep 2020 11:30:00	U	SMPL
ChkStd - 1	ChkStd	24488	7.3536	-	7470A	PPB	02 Sep 2020 11:32:15	U	SMPL
PB131343BL - 1	PBW	-23	0.0242	-	7470A	PPB	02 Sep 2020 11:37:04	U	SMPL
PB131343BS - 1	LCSW	13426	4.0458	-	7470A	PPB	02 Sep 2020 11:39:19	U	SMPL
L3506-15 - 1	OR-02-083120	-251	-0.0440	-	7470A	PPB	02 Sep 2020 11:41:36	U	SMPL
L3506-15DUP - 1	OR-02-083120DUP	-114	-0.0030	-	7470A	PPB	02 Sep 2020 11:43:53	U	SMPL
L3506-15MS - 1	OR-02-083120MS	12540	3.7808	-	7470A	PPB	02 Sep 2020 11:46:10	U	SMPL
L3506-15MSD - 1	OR-02-083120MSD	13846	4.1713	-	7470A	PPB	02 Sep 2020 11:48:27	U	SMPL
L3849-03 - 1	16090	-265	-0.0482	-	7470A	PPB	02 Sep 2020 11:50:43	U	SMPL
CCV30 - 1	CCV30	17485	5.2595	-	7470A	PPB	02 Sep 2020 11:52:59	U	SMPL
CCB30 - 1	CCB30	-188	-0.0252	-	7470A	PPB	02 Sep 2020 11:55:15	U	SMPL
L3849-06 - 1	232	-110	-0.0018	-	7470A	PPB	02 Sep 2020 11:57:30	U	SMPL
L3849-09 - 1	209	-87	0.0050	-	7470A	PPB	02 Sep 2020 11:59:46	U	SMPL
L3850-03 - 1	15203	-73	0.0092	-	7470A	PPB	02 Sep 2020 12:02:01	U	SMPL
L3850-06 - 1	228	-55	0.0146	-	7470A	PPB	02 Sep 2020 12:04:17	U	SMPL
L3851-03 - 1	11995	-63	0.0122	-	7470A	PPB	02 Sep 2020 12:06:33	U	SMPL
L3851-06 - 1	238	-49	0.0164	-	7470A	PPB	02 Sep 2020 12:08:49	U	SMPL
L3851-09 - 1	20058	-44	0.0179	-	7470A	PPB	02 Sep 2020 12:11:06	U	SMPL
L3851-12 - 1	24743	-49	0.0164	-	7470A	PPB	02 Sep 2020 12:13:24	U	SMPL
L3851-15 - 1	11998	-55	0.0146	-	7470A	PPB	02 Sep 2020 12:15:42	U	SMPL
L3851-18 - 1	RBR-78	-39	0.0194	-	7470A	PPB	02 Sep 2020 12:17:58	U	SMPL
CCV31 - 1	CCV31	17415	5.2386	-	7470A	PPB	02 Sep 2020 12:20:14	U	SMPL
CCB31 - 1	CCB31	-118	-0.0042	-	7470A	PPB	02 Sep 2020 12:22:29	U	SMPL
L3852-03 - 1	251378	-100	0.0011	-	7470A	PPB	02 Sep 2020 12:24:46	U	SMPL
L3852-06 - 1	206	-70	0.0101	-	7470A	PPB	02 Sep 2020 12:27:01	U	SMPL
L3852-09 - 1	24179	-59	0.0134	-	7470A	PPB	02 Sep 2020 12:29:17	U	SMPL
L3853-03 - 1	208	-64	0.0119	-	7470A	PPB	02 Sep 2020 12:31:32	U	SMPL
L3853-06 - 1	11934	-56	0.0143	-	7470A	PPB	02 Sep 2020 12:33:48	U	SMPL
L3854-01 - 1	DRUM-1-3	-26	0.0233	-	7470A	PPB	02 Sep 2020 12:36:04	U	SMPL
L3859-04 - 1	TP-1-S	-49	0.0164	-	7470A	PPB	02 Sep 2020 12:38:20	U	SMPL
PB131344BL - 1	PBW	-51	0.0158	-	7470A	PPB	02 Sep 2020 12:43:14	U	SMPL
PB131344BS - 1	LCSW	13133	3.9581	-	7470A	PPB	02 Sep 2020 12:45:31	U	SMPL
L3854-07 - 1	1332-FM648	-159	-0.0165	-	7470A	PPB	02 Sep 2020 12:47:46	U	SMPL
CCV32 - 1	CCV32	17259	5.1919	-	7470A	PPB	02 Sep 2020 12:50:02	U	SMPL
CCB32 - 1	CCB32	-158	-0.0162	-	7470A	PPB	02 Sep 2020 12:52:17	U	SMPL
L3854-07DUP - 1	1332-FM648DUP	-82	0.0065	-	7470A	PPB	02 Sep 2020 12:54:34	U	SMPL
L3854-07MS - 1	1332-FM648MS	15560	4.6839	-	7470A	PPB	02 Sep 2020 12:56:49	U	SMPL
L3854-07MSD - 1	1332-FM648MSD	15495	4.6644	-	7470A	PPB	02 Sep 2020 12:59:05	U	SMPL
PB131329BL - 1	PBW	-232	-0.0383	-	7470A	PPB	02 Sep 2020 13:01:20	U	SMPL
PB131329BS - 1	LCSW	11744	3.5428	-	7470A	PPB	02 Sep 2020 13:03:37	U	SMPL
L3828-08 - 1	GW	-11	0.0278	-	7470A	PPB	02 Sep 2020 13:05:53	U	SMPL
L3854-06 - 1	1332-FM648	3210	0.9909	-	7470A	PPB	02 Sep 2020 13:08:10	U	SMPL
L3854-06MS - 1	1332-FM648MS	15927	4.7936	-	7470A	PPB	02 Sep 2020 13:12:45	U	SMPL
L3854-06MSD - 1	1332-FM648MSD	15774	4.7479	-	7470A	PPB	02 Sep 2020 13:15:01	U	SMPL
CCV33 - 1	CCV33	16673	5.0167	-	7470A	PPB	02 Sep 2020 13:17:18	U	SMPL
CCB33 - 1	CCB33	-122	-0.0054	-	7470A	PPB	02 Sep 2020 13:19:36	U	SMPL
L3858-02 - 1	HAM-WC-L-VB01	2658	0.8259	-	7470A	PPB	02 Sep 2020 13:21:51	U	SMPL
PB131343TB - 1	PB131313TB	-120	-0.0048	-	7470A	PPB	02 Sep 2020 13:24:07	U	SMPL
PB131344TB - 1	PB131315TB	-50	0.0161	-	7470A	PPB	02 Sep 2020 13:26:24	U	SMPL
L3854-06DUP - 1	1332-FM648DUP	3538	1.0890	-	7470A	PPB	02 Sep 2020 13:28:40	U	SMPL
L3506-15LX5 - 1		-101	0.0008	-	7470A	PPB	02 Sep 2020 13:30:56	U	SMPL
L3506-15A - 1		12962	3.9070	-	7470A	PPB	02 Sep 2020 13:33:12	U	SMPL
L3854-07LX5 - 1		-156	-0.0156	-	7470A	PPB	02 Sep 2020 13:35:28	U	SMPL
L3854-07A - 1		13478	4.0613	-	7470A	PPB	02 Sep 2020 13:37:45	U	SMPL
L3854-06LX5 - 1		21	0.0373	-	7470A	PPB	02 Sep 2020 13:40:02	U	SMPL
L3854-06A - 1		16879	5.0783	-	7470A	PPB	02 Sep 2020 13:42:19	U	SMPL
CCV34 - 1	CCV34	17140	5.1563	-	7470A	PPB	02 Sep 2020 13:44:35	U	SMPL
CCB34 - 1	CCB34	-120	-0.0048	-	7470A	PPB	02 Sep 2020 13:46:52	U	SMPL