


LB110803

7470A

INSTRUMENT ID: CV2

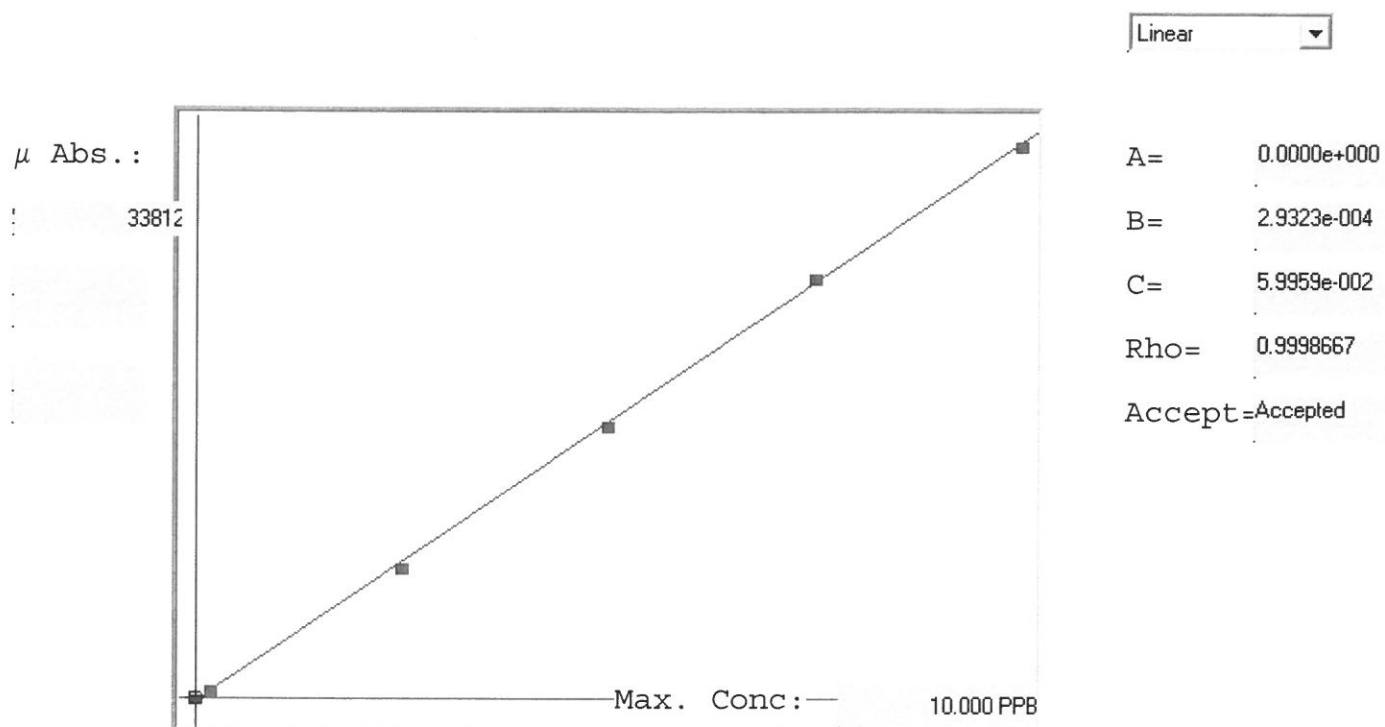

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.052	0.052	-26	0.000	-26				
0.2	0.200	0.214	0.014	527	0.0 %	527				
2.5	2.500	2.419	-0.081	8045	0.0 %	8045				
5.0	5.000	4.946	-0.054	16663	0.0 %	16663				
7.5	7.500	7.593	0.093	25691	0.0 %	25691				
10.0	10.000	9.975	-0.025	33812	0.0 %	33812				

LB110803 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 03 Sep 2020 10:13:42					
Sample ID	Extended ID	μ Abs.	Conc.	Std. Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-26	-	0.0000	7470A	PPB	03 Sep 2020 10:18:22	S	Std
0.2 - 1	50.2	527	-	0.2000	7470A	PPB	03 Sep 2020 10:20:39	S	Std
2.5 - 1	52.5	8045	-	2.5000	7470A	PPB	03 Sep 2020 10:22:56	S	Std
5.0 - 1	55	16663	-	5.0000	7470A	PPB	03 Sep 2020 10:25:13	S	Std
7.5 - 1	57.5	25691	-	7.5000	7470A	PPB	03 Sep 2020 10:27:29	S	Std
10.0 - 1	510	33812	-	10.0000	7470A	PPB	03 Sep 2020 10:37:23	S	Std
ICV96 - 1	ICV96	12495	3.7239	-	7470A	PPB	03 Sep 2020 10:40:06	U	SMPL
ICB96 - 1	ICB96	-273	-0.0201	-	7470A	PPB	03 Sep 2020 10:42:20	U	SMPL
CCV41 - 1	CCV41	16599	4.9273	-	7470A	PPB	03 Sep 2020 10:44:37	U	SMPL
CCB41 - 1	CCB41	-259	-0.0160	-	7470A	PPB	03 Sep 2020 10:46:52	U	SMPL
CRA - 1	CRA	480	0.2007	-	7470A	PPB	03 Sep 2020 10:49:08	U	SMPL
HighStd - 1	HighStd	34011	10.0331	-	7470A	PPB	03 Sep 2020 10:51:23	U	SMPL
ChkStd - 1	ChkStd	24359	7.2028	-	7470A	PPB	03 Sep 2020 10:53:39	U	SMPL
PB131376BL - 1	PBW	-370	-0.0485	-	7470A	PPB	03 Sep 2020 10:55:57	U	SMPL
PB131376BS - 1	LCSW	11961	3.5673	-	7470A	PPB	03 Sep 2020 11:01:13	U	SMPL
L3866-05 - 1	OK-03-090120	-244	-0.0116	-	7470A	PPB	03 Sep 2020 11:03:29	U	SMPL
L3866-05DUP - 1	OK-03-090120DUP	-99	0.0309	-	7470A	PPB	03 Sep 2020 11:05:46	U	SMPL
L3866-05MS - 1	OK-03-090120MS	10919	3.2618	-	7470A	PPB	03 Sep 2020 11:08:03	U	SMPL
L3866-05MSD - 1	OK-03-090120MSD	11616	3.4661	-	7470A	PPB	03 Sep 2020 11:10:20	U	SMPL
L3876-01 - 1	1500	-195	0.0028	-	7470A	PPB	03 Sep 2020 11:12:35	U	SMPL
CCV42 - 1	CCV42	16522	4.9047	-	7470A	PPB	03 Sep 2020 11:14:51	U	SMPL
CCB42 - 1	CCB42	-235	-0.0090	-	7470A	PPB	03 Sep 2020 11:17:06	U	SMPL
L3876-02 - 1	1494	-87	0.0344	-	7470A	PPB	03 Sep 2020 11:19:23	U	SMPL
L3876-03 - 1	1449	-79	0.0368	-	7470A	PPB	03 Sep 2020 11:21:38	U	SMPL
L3876-04 - 1	1447	-67	0.0403	-	7470A	PPB	03 Sep 2020 11:23:54	U	SMPL
L3876-06 - 1	1458-62	-47	0.0462	-	7470A	PPB	03 Sep 2020 11:26:10	U	SMPL
L3876-08 - 1	1495-96	-40	0.0482	-	7470A	PPB	03 Sep 2020 11:28:25	U	SMPL
L3876-11 - 1	1451-52	-46	0.0465	-	7470A	PPB	03 Sep 2020 11:30:42	U	SMPL
L3876-13 - 1	VNJ-215	-32	0.0506	-	7470A	PPB	03 Sep 2020 11:32:58	U	SMPL
L3878-02 - 1	Z3-IDW-SOIL-0820	-42	0.0476	-	7470A	PPB	03 Sep 2020 11:35:15	U	SMPL
L3882-01 - 1	WC-1	-35	0.0497	-	7470A	PPB	03 Sep 2020 11:37:32	U	SMPL
L3882-02 - 1	WC-2	-31	0.0509	-	7470A	PPB	03 Sep 2020 11:39:49	U	SMPL
CCV43 - 1	CCV43	15924	4.7294	-	7470A	PPB	03 Sep 2020 11:42:04	U	SMPL
CCB43 - 1	CCB43	-163	0.0122	-	7470A	PPB	03 Sep 2020 11:44:20	U	SMPL
L3882-03 - 1	WC-3	-41	0.0479	-	7470A	PPB	03 Sep 2020 11:46:36	U	SMPL
PB131377BS - 1	LCSW	12492	3.7230	-	7470A	PPB	03 Sep 2020 11:54:07	U	SMPL
L3874-01 - 1	31216	-175	0.0086	-	7470A	PPB	03 Sep 2020 11:56:22	U	SMPL
L3874-01DUP - 1	31216DUP	-63	0.0415	-	7470A	PPB	03 Sep 2020 12:01:27	U	SMPL
L3874-01MS - 1	31216MS	12452	3.7113	-	7470A	PPB	03 Sep 2020 12:06:21	U	SMPL
L3874-01MSD - 1	31216MSD	12717	3.7890	-	7470A	PPB	03 Sep 2020 12:08:38	U	SMPL
L3876-14 - 1	1576	-174	0.0089	-	7470A	PPB	03 Sep 2020 12:10:55	U	SMPL
PB131377BL - 1	PBW	-65	0.0409	-	7470A	PPB	03 Sep 2020 12:13:11	U	SMPL
CCV44 - 1	CCV44	17360	5.1505	-	7470A	PPB	03 Sep 2020 12:15:27	U	SMPL
CCB44 - 1	CCB44	-197	0.0022	-	7470A	PPB	03 Sep 2020 12:17:43	U	SMPL
PB131376TB - 1	PB131249TB	-53	0.0444	-	7470A	PPB	03 Sep 2020 12:19:59	U	SMPL
PB131377TB - 1	PB131252TB	-19	0.0544	-	7470A	PPB	03 Sep 2020 12:22:14	U	SMPL
L3866-05LX5 - 1		-33	0.0503	-	7470A	PPB	03 Sep 2020 12:24:30	U	SMPL
L3866-05A - 1		12310	3.6696	-	7470A	PPB	03 Sep 2020 12:26:45	U	SMPL
L3874-01LX5 - 1		-182	0.0066	-	7470A	PPB	03 Sep 2020 12:29:01	U	SMPL
L3874-01A - 1		12187	3.6336	-	7470A	PPB	03 Sep 2020 12:31:17	U	SMPL
CCV45 - 1	CCV45	16176	4.8033	-	7470A	PPB	03 Sep 2020 12:33:33	U	SMPL
CCB45 - 1	CCB45	-188	0.0048	-	7470A	PPB	03 Sep 2020 12:35:51	U	SMPL