


LB110815

7471B

INSTRUMENT ID: CVI

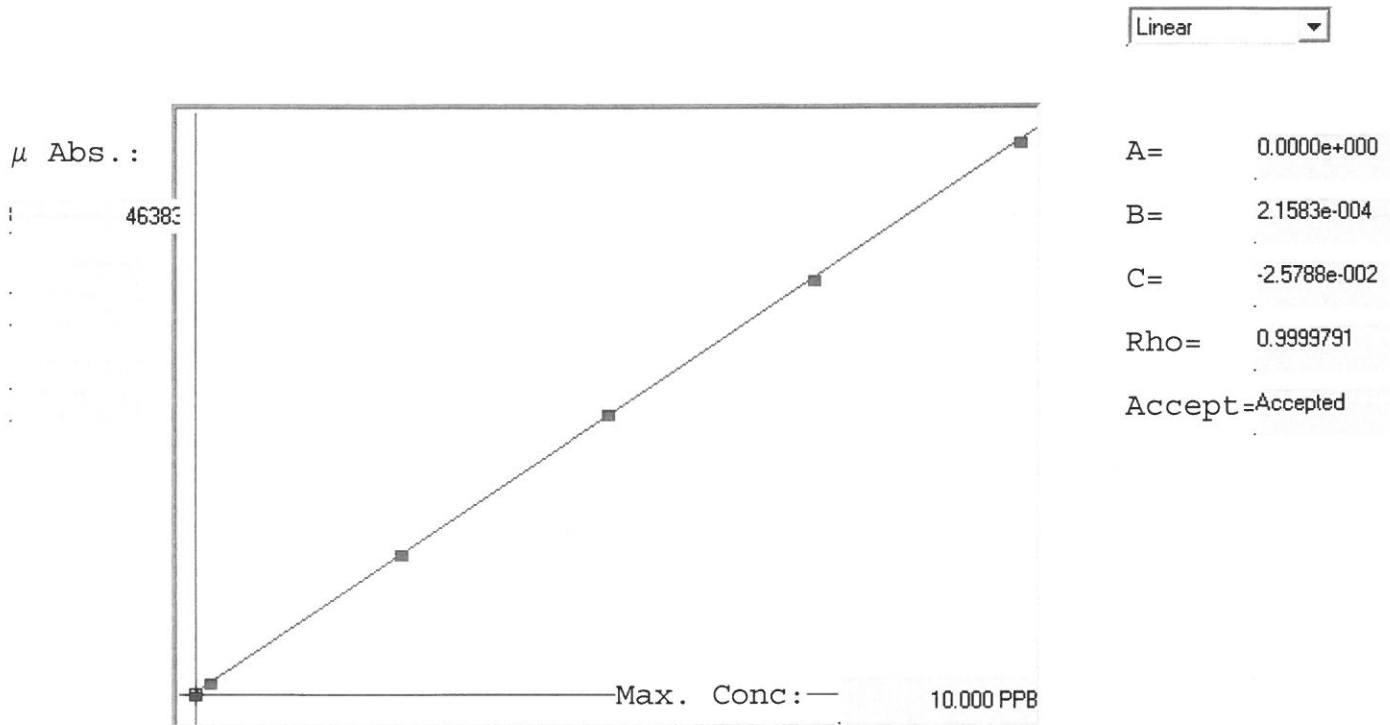

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.030	-0.030	-20	0.000	-20				
0.2	0.200	0.194	-0.006	1019	0.0 %	1019				
2.5	2.500	2.530	0.030	11840	0.0 %	11840				
5.0	5.000	5.035	0.035	23446	0.0 %	23446				
7.5	7.500	7.487	-0.013	34808	0.0 %	34808				
10.0	10.000	9.985	-0.015	46383	0.0 %	46383				

LB110815 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 03 Sep 2020 15:17:23

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-20	-	0.0000	7471B	PPB	03 Sep 2020 15:18:20	S	Std
0.2 - 1	50.2	1019	-	0.2000	7471B	PPB	03 Sep 2020 15:20:38	S	Std
2.5 - 1	52.5	11840	-	2.5000	7471B	PPB	03 Sep 2020 15:22:56	S	Std
5.0 - 1	55	23446	-	5.0000	7471B	PPB	03 Sep 2020 15:25:12	S	Std
7.5 - 1	57.5	34808	-	7.5000	7471B	PPB	03 Sep 2020 15:27:29	S	Std
10.0 - 1	51.8	46383	-	10.0000	7471B	PPB	03 Sep 2020 15:32:20	S	Std
ICV98 - 1	ICV98	19023	4.0799	-	7471B	PPB	03 Sep 2020 15:35:06	U	SMPL
ICB98 - 1	ICB98	-49	-0.0364	-	7471B	PPB	03 Sep 2020 15:37:21	U	SMPL
CCV49 - 1	CCV49	24157	5.1880	-	7471B	PPB	03 Sep 2020 15:39:38	U	SMPL
CCB49 - 1	CCB49	-204	-0.0698	-	7471B	PPB	03 Sep 2020 15:41:53	U	SMPL
CRA - 1	CRA	1078	0.2069	-	7471B	PPB	03 Sep 2020 15:44:10	U	SMPL
HighStd - 1	HighStd	45949	9.8913	-	7471B	PPB	03 Sep 2020 15:46:25	U	SMPL
ChkStd - 1	ChkStd	33744	7.2571	-	7471B	PPB	03 Sep 2020 15:48:40	U	SMPL
PB131398BL - 1	PBS	-296	-0.0897	-	7471B	PPB	03 Sep 2020 15:50:57	U	SMPL
PB131398BS - 1	LCSS	16607	3.5585	-	7471B	PPB	03 Sep 2020 15:53:15	U	SMPL
L3871-01 - 1	TR-05-090220	1823	0.3677	-	7471B	PPB	03 Sep 2020 16:00:24	U	SMPL
L3871-01DUP - 1	TR-05-090220DUP	1664	0.3334	-	7471B	PPB	03 Sep 2020 16:02:41	U	SMPL
L3871-01MS - 1	TR-05-090220MS	19056	4.0870	-	7471B	PPB	03 Sep 2020 16:04:57	U	SMPL
L3871-01MSD - 1	TR-05-090220MSD	20682	4.4380	-	7471B	PPB	03 Sep 2020 16:07:15	U	SMPL
L3877-02 - 1	TP-1	13534	2.8952	-	7471B	PPB	03 Sep 2020 16:09:31	U	SMPL
CCV50 - 1	CCV50	24513	5.2648	-	7471B	PPB	03 Sep 2020 16:11:48	U	SMPL
CCB50 - 1	CCB50	-158	-0.0599	-	7471B	PPB	03 Sep 2020 16:14:05	U	SMPL
L3877-07 - 1	TP-2	25798	5.5422	-	7471B	PPB	03 Sep 2020 16:16:21	U	SMPL
L3877-12 - 1	TP-3	124066	26.7513	-	7471B	PPB	03 Sep 2020 16:18:36	U	SMPL
L3877-17 - 1	TP-4	6543	1.3864	-	7471B	PPB	03 Sep 2020 16:20:53	U	SMPL
L3888-02 - 1	9-2-TP-1	5025	1.0588	-	7471B	PPB	03 Sep 2020 16:23:12	U	SMPL
L3888-06 - 1	9-2-TP-2	5657	1.1952	-	7471B	PPB	03 Sep 2020 16:25:28	U	SMPL
L3888-10 - 1	9-2-TP-3	1904	0.3852	-	7471B	PPB	03 Sep 2020 16:27:46	U	SMPL
L3888-14 - 1	9-2-TP-4	2505	0.5149	-	7471B	PPB	03 Sep 2020 16:30:03	U	SMPL
L3896-01 - 1	WC-1	1923	0.3893	-	7471B	PPB	03 Sep 2020 16:32:20	U	SMPL
L3871-01LX5 - 1		216	0.0208	-	7471B	PPB	03 Sep 2020 16:34:37	U	SMPL
L3871-01A - 1		20703	4.4425	-	7471B	PPB	03 Sep 2020 16:36:52	U	SMPL
CCV51 - 1	CCV51	24601	5.2838	-	7471B	PPB	03 Sep 2020 16:39:08	U	SMPL
CCB51 - 1	CCB51	-117	-0.0510	-	7471B	PPB	03 Sep 2020 16:41:23	U	SMPL
L3877-12DLX5 - 1		25114	5.3945	-	7471B	PPB	03 Sep 2020 16:43:40	U	SMPL
CCV52 - 1	CCV52	24574	5.2780	-	7471B	PPB	03 Sep 2020 16:45:56	U	SMPL
CCB52 - 1	CCB52	-146	-0.0573	-	7471B	PPB	03 Sep 2020 16:48:12	U	SMPL