


LB 110836

ISM02.4

INSTRUMENT ID: CV2

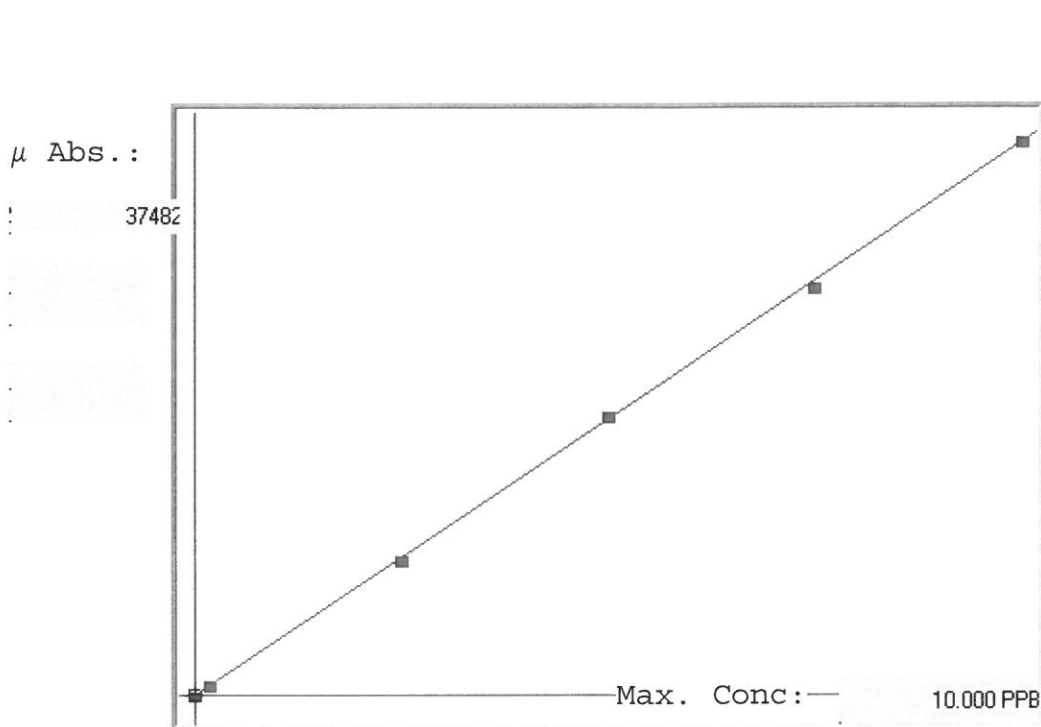

Linear

A= 0.0000e+000

B= 2.6754e-004

C= 1.6477e-002

Rho= 0.9998763

Accept=Accepted

slope
Y=mx+c

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.016	0.016	-3	0.000	-3					1
0.05	0.050					159					-1
0.20	0.200	0.199	-0.001	684	0.0 %	684					-1
2.50	2.500	2.464	-0.036	9149	0.0 %	9149					2
5.00	5.000	5.079	0.079	18921	0.0 %	18921					-1
7.50	7.500	7.397	-0.103	27588	0.0 %	27588					0
10.0	10.000	10.045	0.045	37482	0.0 %	37482					

LB110836
INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0.0	-3	-		0 ISM02.4	PPB	9/4/2020 14:53	Std
	0.2 S0.2	684	-		0.2 ISM02.4	PPB	9/4/2020 14:55	Std
	2.5 S2.5	9149	-		2.5 ISM02.4	PPB	9/4/2020 15:00	Std
	5 S5.0	18921	-		5 ISM02.4	PPB	9/4/2020 15:02	Std
	7.5 S7.5	27588	-		7.5 ISM02.4	PPB	9/4/2020 15:05	Std
	10 S10.0	37482	-		10 ISM02.4	PPB	9/4/2020 15:07	Std
ICV	ICV	14494	3.8942 -		ISM02.4	PPB	9/4/2020 15:10	SMPL
ICB	ICB	-158	-0.0258 -		ISM02.4	PPB	9/4/2020 15:12	SMPL
CCV063	CCV063	19849	5.3269 -		ISM02.4	PPB	9/4/2020 15:14	SMPL
CCB063	CCB063	-165	-0.0277 -		ISM02.4	PPB	9/4/2020 15:16	SMPL
PB131444BL	PBW444	-41	0.0055 -		ISM02.4	PPB	9/4/2020 15:19	SMPL
L3844-23	MCOAE8	-87	-0.0068 -		ISM02.4	PPB	9/4/2020 15:21	SMPL
L3844-24	MCOAE9	-87	-0.0068 -		ISM02.4	PPB	9/4/2020 15:23	SMPL
PB131445BL	PBW445	-38	0.0063 -		ISM02.4	PPB	9/4/2020 15:25	SMPL
L3845-08	MCOAE7	-63	-0.0004 -		ISM02.4	PPB	9/4/2020 15:28	SMPL
L3845-09	MCOAF0	-59	0.0007 -		ISM02.4	PPB	9/4/2020 15:30	SMPL
CCV064	CCV064	18104	4.8601 -		ISM02.4	PPB	9/4/2020 15:32	SMPL
CCB064	CCB064	-139	-0.0207 -		ISM02.4	PPB	9/4/2020 15:34	SMPL