


LB110863

7471B

INSTRUMENT ID: CV1

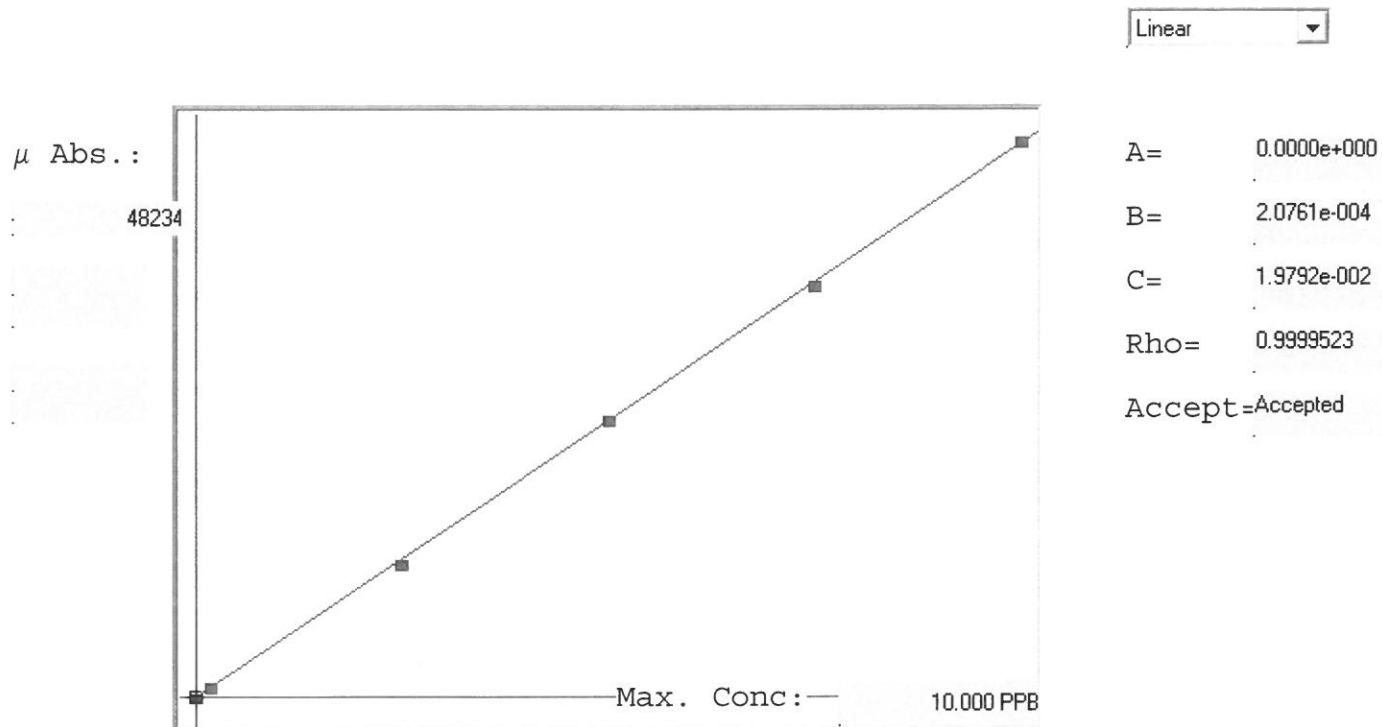

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.028	0.028	40	0.000	40				
0.2	0.200	0.222	0.022	976	0.0 %	976				
2.5	2.500	2.437	-0.063	11642	0.0 %	11642				
5.0	5.000	5.013	0.013	24053	0.0 %	24053				
7.5	7.500	7.466	-0.034	35864	0.0 %	35864				
10.0	10.000	10.034	0.034	48234	0.0 %	48234				

LB110863 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 08 Sep 2020 14:05:32					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	40	-	0.00007471B	PPB		08 Sep 2020 14:07:27	S	Std
0.2 - 1	50.2	976	-	0.20007471B	PPB		08 Sep 2020 14:09:44	S	Std
2.5 - 1	52.5	11642	-	2.50007471B	PPB		08 Sep 2020 14:12:01	S	Std
5.0 - 1	55	24053	-	5.00007471B	PPB		08 Sep 2020 14:14:18	S	Std
7.5 - 1	57.5	35864	-	7.50007471B	PPB		08 Sep 2020 14:16:35	S	Std
10.0 - 1	510	48234	-	10.00007471B	PPB		08 Sep 2020 14:18:52	S	Std
ICV03 - 1	ICV03	18583	3.8778	-7471B	PPB		08 Sep 2020 14:21:38	U	SMPL
ICB03 - 1	ICB03	-60	0.0073	-7471B	PPB		08 Sep 2020 14:23:53	U	SMPL
CCV68 - 1	CCV68	24642	5.1357	-7471B	PPB		08 Sep 2020 14:26:09	U	SMPL
CCB68 - 1	CCB68	-78	0.0036	-7471B	PPB		08 Sep 2020 14:28:24	U	SMPL
CRA - 1	CRA	992	0.2257	-7471B	PPB		08 Sep 2020 14:30:41	U	SMPL
HighStd - 1	HighStd	47542	9.8900	-7471B	PPB		08 Sep 2020 14:32:55	U	SMPL
ChkStd - 1	ChkStd	34392	7.1599	-7471B	PPB		08 Sep 2020 14:35:11	U	SMPL
PB131460BL - 1	PBS	-249	-0.0319	-7471B	PPB		08 Sep 2020 14:37:29	U	SMPL
PB131460BS - 1	LCSS	18566	3.8743	-7471B	PPB		08 Sep 2020 14:39:46	U	SMPL
L3808-05 - 1	PAV-B44-090320-0-10	21756	4.5366	-7471B	PPB		08 Sep 2020 14:42:04	U	SMPL
L3808-07 - 1	PAV-B44-090320-10-20	813	0.1886	-7471B	PPB		08 Sep 2020 14:44:21	U	SMPL
L3808-09 - 1	PAV-B44-090320-DP	4515	0.9572	-7471B	PPB		08 Sep 2020 14:46:39	U	SMPL
L3872-01 - 1	BU-03-090420	1507	0.3327	-7471B	PPB		08 Sep 2020 14:48:56	U	SMPL
L3915-13 - 1	WC-A2-10-14-C	80424	16.7167	-7471B	PPB		08 Sep 2020 14:51:11	U	SMPL
CCV69 - 1	CCV69	23847	4.9707	-7471B	PPB		08 Sep 2020 14:53:27	U	SMPL
CCB69 - 1	CCB69	-72	0.0048	-7471B	PPB		08 Sep 2020 14:55:45	U	SMPL
L3916-01 - 1	WC-1	3666	0.7809	-7471B	PPB		08 Sep 2020 14:58:02	U	SMPL
L3919-02 - 1	TP-10	5418	1.1446	-7471B	PPB		08 Sep 2020 15:00:18	U	SMPL
L3919-05 - 1	TP-11	2373	0.5125	-7471B	PPB		08 Sep 2020 15:02:33	U	SMPL
L3919-08 - 1	TP-12	2581	0.5556	-7471B	PPB		08 Sep 2020 15:04:49	U	SMPL
L3919-11 - 1	TP-13	2283	0.4938	-7471B	PPB		08 Sep 2020 15:07:05	U	SMPL
L3919-14 - 1	TP-14	4818	1.0201	-7471B	PPB		08 Sep 2020 15:09:22	U	SMPL
L3919-17 - 1	TP-15	3620	0.7713	-7471B	PPB		08 Sep 2020 15:11:38	U	SMPL
L3919-17DUP - 1	TP-15DUP	3632	0.7738	-7471B	PPB		08 Sep 2020 15:13:55	U	SMPL
L3919-17MS - 1	TP-15MS	23918	4.9854	-7471B	PPB		08 Sep 2020 15:16:12	U	SMPL
L3919-17MSD - 1	TP-15MSD	24042	5.0112	-7471B	PPB		08 Sep 2020 15:18:27	U	SMPL
CCV70 - 1	CCV70	25073	5.2252	-7471B	PPB		08 Sep 2020 15:20:44	U	SMPL
CCB70 - 1	CCB70	-35	0.0125	-7471B	PPB		08 Sep 2020 15:23:00	U	SMPL
L3919-17LX5 - 1		800	0.1859	-7471B	PPB		08 Sep 2020 15:25:16	U	SMPL
L3919-17A - 1		23959	4.9939	-7471B	PPB		08 Sep 2020 15:27:31	U	SMPL
L3915-13DLX5 - 1		16285	3.4007	-7471B	PPB		08 Sep 2020 15:29:47	U	SMPL
CCV71 - 1	CCV71	24553	5.1173	-7471B	PPB		08 Sep 2020 15:32:03	U	SMPL
CCB71 - 1	CCB71	-39	0.0117	-7471B	PPB		08 Sep 2020 15:34:20	U	SMPL