


LB 110870

7470A

INSTRUMENT ID: CV1

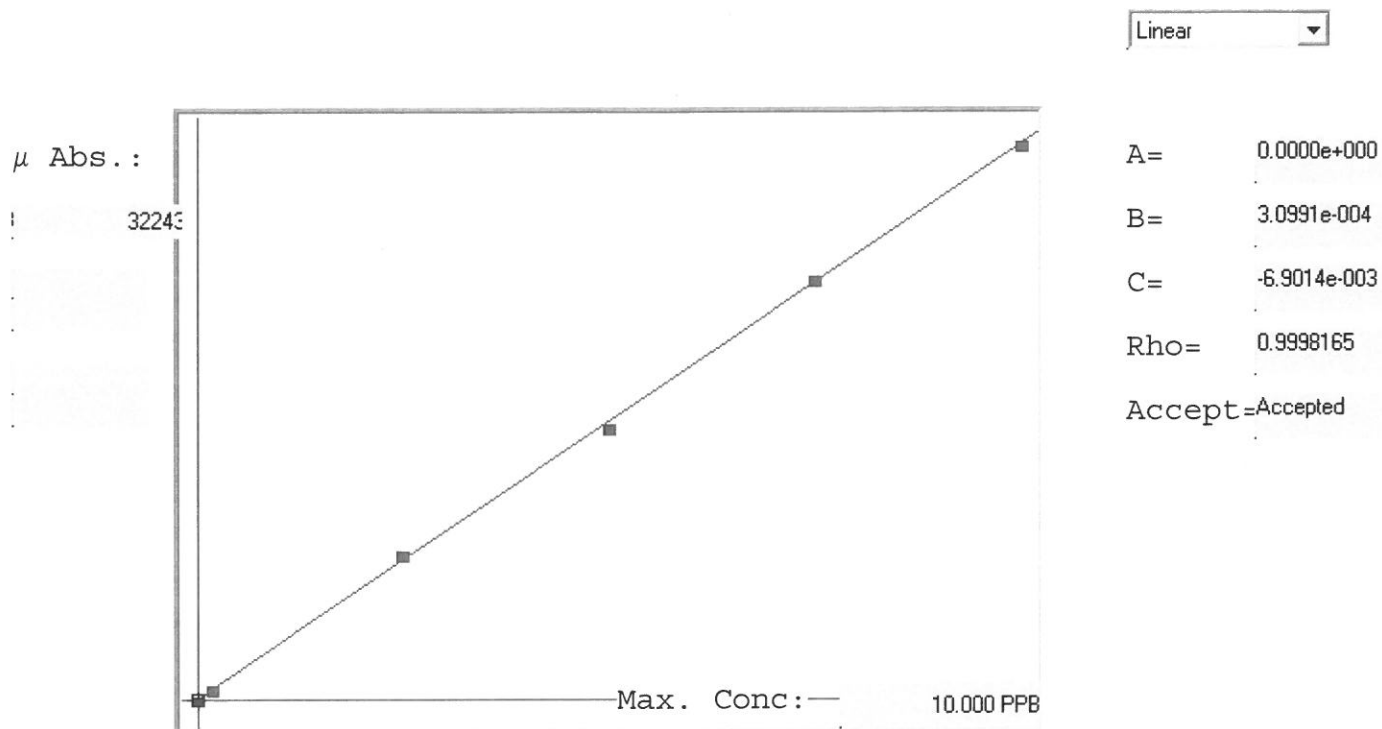

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.009	-0.009	-8	0.000	-8				
0.2	0.200	0.185	-0.015	619	0.0 %	619				
2.5	2.500	2.597	0.097	8403	0.0 %	8403				
5.0	5.000	4.875	-0.125	15753	0.0 %	15753				
7.5	7.500	7.566	0.066	24437	0.0 %	24437				
10.0	10.000	9.986	-0.014	32243	0.0 %	32243				

LB110870 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 09 Sep 2020 09:50:23					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-8	-	0.0000	7470A	PPB	09 Sep 2020 09:54:02	S	Std
0.2 - 1	50.2	619	-	0.2000	7470A	PPB	09 Sep 2020 09:56:19	S	Std
2.5 - 1	52.5	8403	-	2.5000	7470A	PPB	09 Sep 2020 09:58:36	S	Std
5.0 - 1	55	15753	-	5.0000	7470A	PPB	09 Sep 2020 10:00:53	S	Std
7.5 - 1	57.5	24437	-	7.5000	7470A	PPB	09 Sep 2020 10:03:09	S	Std
10.0 - 1	510	32243	-	10.0000	7470A	PPB	09 Sep 2020 10:05:26	S	Std
ICV04 - 1	ICV04	11763	3.6386	-7470A	PPB	09 Sep 2020 10:08:11	U	SMPL	
ICB04 - 1	ICB04	-214	-0.0732	-7470A	PPB	09 Sep 2020 10:10:26	U	SMPL	
CCV72 - 1	CCV72	15994	4.9498	-7470A	PPB	09 Sep 2020 10:15:07	U	SMPL	
CCB72 - 1	CCB72	-198	-0.0683	-7470A	PPB	09 Sep 2020 10:17:22	U	SMPL	
CRA - 1	CRA	553	0.1645	-7470A	PPB	09 Sep 2020 10:19:38	U	SMPL	
HighStd - 1	HighStd	31116	9.6363	-7470A	PPB	09 Sep 2020 10:21:53	U	SMPL	
ChkStd - 1	ChkStd	21839	6.7613	-7470A	PPB	09 Sep 2020 10:24:09	U	SMPL	
PB131476BL - 1	PBW	-301	-0.1002	-7470A	PPB	09 Sep 2020 10:26:26	U	SMPL	
PB131476BS - 1	LCSW	10852	3.3563	-7470A	PPB	09 Sep 2020 10:28:44	U	SMPL	
L3808-11 - 1	PAV-B44-090320-0-10	-148	-0.0528	-7470A	PPB	09 Sep 2020 10:31:00	U	SMPL	
L3808-11DUP - 1	PAV-B44-090320-0-10DUP	-41	-0.0196	-7470A	PPB	09 Sep 2020 10:33:17	U	SMPL	
L3808-11MS - 1	PAV-B44-090320-0-10MS	11814	3.6544	-7470A	PPB	09 Sep 2020 10:35:34	U	SMPL	
L3808-11MSD - 1	PAV-B44-090320-0-10MSD	12551	3.8828	-7470A	PPB	09 Sep 2020 10:37:51	U	SMPL	
L3808-13 - 1	PAV-B44-090320-10-20	-194	-0.0670	-7470A	PPB	09 Sep 2020 10:40:06	U	SMPL	
CCV73 - 1	CCV73	15983	4.9464	-7470A	PPB	09 Sep 2020 10:42:22	U	SMPL	
CCB73 - 1	CCB73	-193	-0.0667	-7470A	PPB	09 Sep 2020 10:44:37	U	SMPL	
L3808-14 - 1	PAV-B44-090320-DP	-54	-0.0236	-7470A	PPB	09 Sep 2020 10:46:54	U	SMPL	
L3872-04 - 1	BU-03-090420	-34	-0.0174	-7470A	PPB	09 Sep 2020 10:49:10	U	SMPL	
L3915-02 - 1	WC-A1-0-4-C	-36	-0.0181	-7470A	PPB	09 Sep 2020 10:51:25	U	SMPL	
L3915-06 - 1	WC-PME-0-5-C	-22	-0.0137	-7470A	PPB	09 Sep 2020 10:53:40	U	SMPL	
L3915-10 - 1	WC-B2-0-3.5-C	-18	-0.0125	-7470A	PPB	09 Sep 2020 10:55:56	U	SMPL	
L3915-14 - 1	WC-A2-10-14-C	288	0.0824	-7470A	PPB	09 Sep 2020 10:58:12	U	SMPL	
L3926-01 - 1	BR-1	-58	-0.0249	-7470A	PPB	09 Sep 2020 11:00:29	U	SMPL	
PB131476TB - 1	PB131450TB	46	0.0074	-7470A	PPB	09 Sep 2020 11:02:46	U	SMPL	
L3808-11LX5 - 1		16	-0.0019	-7470A	PPB	09 Sep 2020 11:05:04	U	SMPL	
L3808-11A - 1		11798	3.6494	-7470A	PPB	09 Sep 2020 11:07:19	U	SMPL	
CCV74 - 1	CCV74	15396	4.7645	-7470A	PPB	09 Sep 2020 11:09:35	U	SMPL	
CCB74 - 1	CCB74	-175	-0.0611	-7470A	PPB	09 Sep 2020 11:11:50	U	SMPL	