


LB110892

7470A

INSTRUMENT ID: CV1

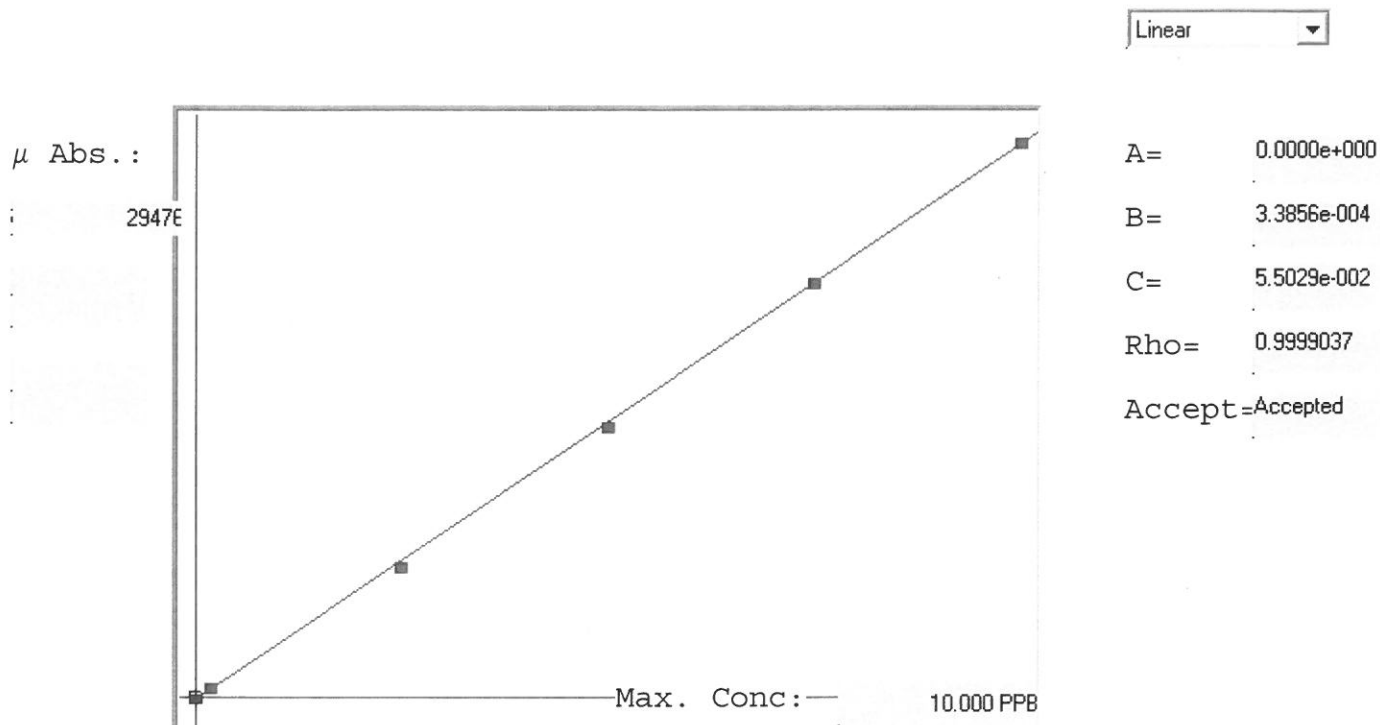

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.057	0.057	6	0.000	6				
0.2	0.200	0.232	0.032	522	0.0 %	522				
2.5	2.500	2.415	-0.085	6971	0.0 %	6971				
5.0	5.000	4.947	-0.053	14448	0.0 %	14448				
7.5	7.500	7.515	0.015	22034	0.0 %	22034				
10.0	10.000	10.035	0.035	29476	0.0 %	29476				

LB110892 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 10 Sep 2020 10:50:32					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	6	-	0.00007470A	PPB		10 Sep 2020 10:57:07	S	Std
0.2 - 1	50.2	522	-	0.20007470A	PPB		10 Sep 2020 10:59:24	S	Std
2.5 - 1	52.5	6971	-	2.50007470A	PPB		10 Sep 2020 11:01:41	S	Std
5.0 - 1	55	14448	-	5.00007470A	PPB		10 Sep 2020 11:03:58	S	Std
7.5 - 1	57.5	22034	-	7.50007470A	PPB		10 Sep 2020 11:06:14	S	Std
10.0 - 1	510	29476	-	10.00007470A	PPB		10 Sep 2020 11:11:09	S	Std
ICV06 - 1	ICV06	11604	3.9837	-7470A	PPB		10 Sep 2020 11:13:49	U	SMPL
ICB06 - 1	ICB06	-210	-0.0161	-7470A	PPB		10 Sep 2020 11:16:05	U	SMPL
CCV80 - 1	CCV80	15733	5.3816	-7470A	PPB		10 Sep 2020 11:18:21	U	SMPL
CCB80 - 1	CCB80	-208	-0.0154	-7470A	PPB		10 Sep 2020 11:20:36	U	SMPL
CRA - 1	CRA	518	0.2304	-7470A	PPB		10 Sep 2020 11:22:53	U	SMPL
HighStd - 1	HighStd	31102	10.5850	-7470A	PPB		10 Sep 2020 11:25:08	U	SMPL
ChkStd - 1	ChkStd	21511	7.3379	-7470A	PPB		10 Sep 2020 11:27:23	U	SMPL
PB131504BL - 1	PBW	-313	-0.0509	-7470A	PPB		10 Sep 2020 11:29:41	U	SMPL
PB131504BS - 1	LCSW	10395	3.5744	-7470A	PPB		10 Sep 2020 11:31:58	U	SMPL
L3870-05 - 1	SU-04-090820	-189	-0.0090	-7470A	PPB		10 Sep 2020 11:34:15	U	SMPL
L3870-05DUP - 1	SU-04-090820DUP	-78	0.0286	-7470A	PPB		10 Sep 2020 11:36:32	U	SMPL
L3870-05MS - 1	SU-04-090820MS	11245	3.8622	-7470A	PPB		10 Sep 2020 11:38:49	U	SMPL
L3870-05MSD - 1	SU-04-090820MSD	12417	4.2590	-7470A	PPB		10 Sep 2020 11:41:07	U	SMPL
L3931-02 - 1	SP-1-1	-181	-0.0063	-7470A	PPB		10 Sep 2020 11:43:23	U	SMPL
CCV81 - 1	CCV81	15179	5.1941	-7470A	PPB		10 Sep 2020 11:45:39	U	SMPL
CCB81 - 1	CCB81	-194	-0.0107	-7470A	PPB		10 Sep 2020 11:47:54	U	SMPL
L3931-04 - 1	SP-1-2	-44	0.0401	-7470A	PPB		10 Sep 2020 11:50:11	U	SMPL
L3932-02 - 1	VNJ-218	-9	0.0520	-7470A	PPB		10 Sep 2020 11:52:26	U	SMPL
L3939-04 - 1	PAV-B41-090820-0-10	-18	0.0489	-7470A	PPB		10 Sep 2020 11:54:41	U	SMPL
PB131511BL - 1	PBW	-6	0.0530	-7470A	PPB		10 Sep 2020 11:56:56	U	SMPL
PB131511BS - 1	LCSW	11053	3.7972	-7470A	PPB		10 Sep 2020 11:59:13	U	SMPL
L3808-03 - 1	FIELD-BLANK	-194	-0.0107	-7470A	PPB		10 Sep 2020 12:01:29	U	SMPL
L3939-07 - 1	PAV-B44-090820-GW	700	0.2920	-7470A	PPB		10 Sep 2020 12:08:40	U	SMPL
L3939-07DUP - 1	PAV-B44-090820-GWDUP	554	0.2426	-7470A	PPB		10 Sep 2020 12:10:56	U	SMPL
L3939-07MS - 1	PAV-B44-090820-GWMS	13793	4.7248	-7470A	PPB		10 Sep 2020 12:13:13	U	SMPL
L3939-07MSD - 1	PAV-B44-090820-GWMSD	14031	4.8054	-7470A	PPB		10 Sep 2020 12:15:29	U	SMPL
CCV82 - 1	CCV82	14910	5.1030	-7470A	PPB		10 Sep 2020 12:17:44	U	SMPL
CCB82 - 1	CCB82	-95	0.0229	-7470A	PPB		10 Sep 2020 12:20:01	U	SMPL
L3939-08 - 1	PAV-B44-090820-GW	-27	0.0459	-7470A	PPB		10 Sep 2020 12:22:17	U	SMPL
PB131504TB - 1	PB131487TB	18	0.0611	-7470A	PPB		10 Sep 2020 12:24:32	U	SMPL
L3870-05LX5 - 1		-14	0.0503	-7470A	PPB		10 Sep 2020 12:26:48	U	SMPL
L3870-05A - 1		11516	3.9539	-7470A	PPB		10 Sep 2020 12:29:03	U	SMPL
L3939-07LX5 - 1		48	0.0713	-7470A	PPB		10 Sep 2020 12:31:19	U	SMPL
L3939-07A - 1		12629	4.3307	-7470A	PPB		10 Sep 2020 12:33:35	U	SMPL
CCV83 - 1	CCV83	14007	4.7973	-7470A	PPB		10 Sep 2020 12:35:51	U	SMPL
CCB83 - 1	CCB83	-83	0.0269	-7470A	PPB		10 Sep 2020 12:38:09	U	SMPL