


LB110915

7470A

INSTRUMENT ID: CV1

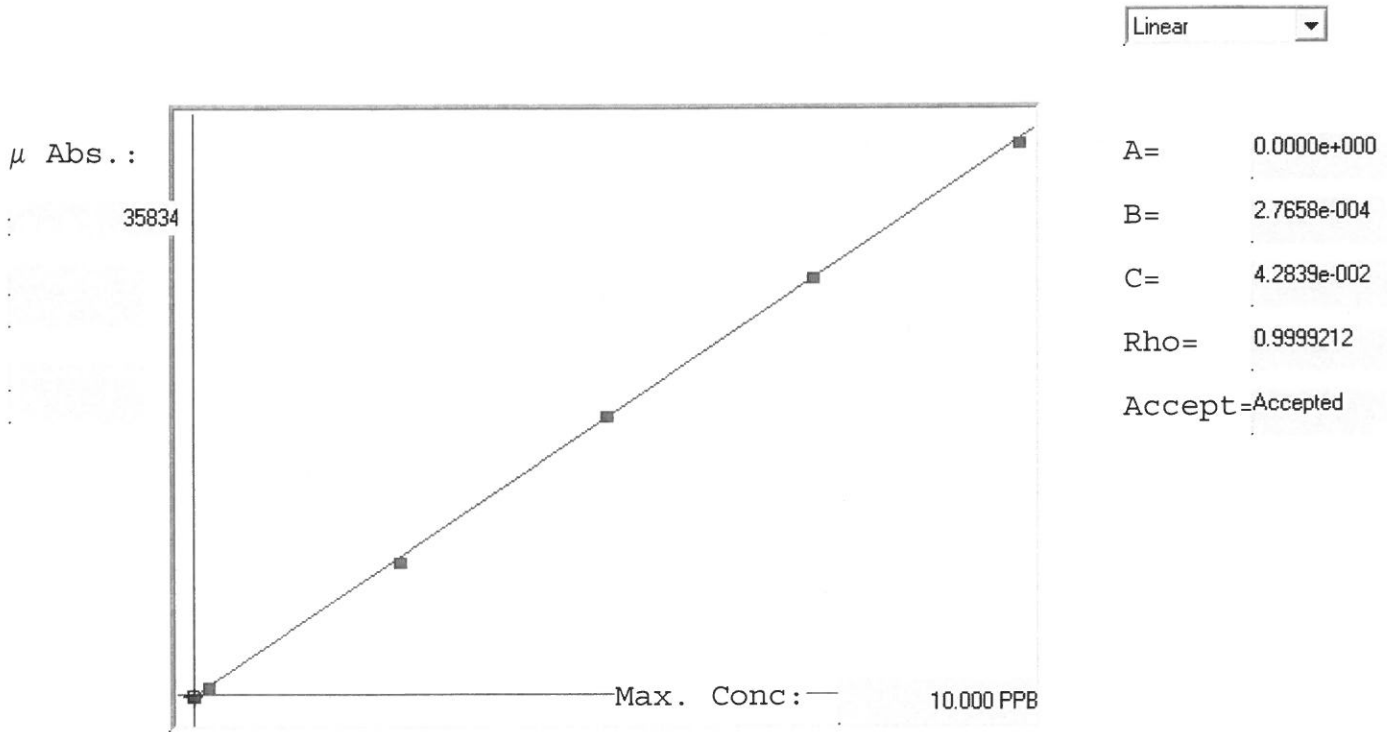

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.006	-0.006	-176	0.000	-176				
0.2	0.200	0.214	0.014	620	0.0 %	620				
2.5	2.500	2.433	-0.067	8642	0.0 %	8642				
5.0	5.000	5.069	0.069	18171	0.0 %	18171				
7.5	7.500	7.536	0.036	27093	0.0 %	27093				
10.0	10.000	9.954	-0.046	35834	0.0 %	35834				

LB110915 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Sep 2020 10:41:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-176	-	0.0000	7470A	PPB	11 Sep 2020 10:48:55	S	Std
0.2 - 1	50.2	620	-	0.2000	7470A	PPB	11 Sep 2020 10:51:13	S	Std
2.5 - 1	52.5	8642	-	2.5000	7470A	PPB	11 Sep 2020 10:53:30	S	Std
5.0 - 1	55	18171	-	5.0000	7470A	PPB	11 Sep 2020 10:55:47	S	Std
7.5 - 1	57.5	27093	-	7.5000	7470A	PPB	11 Sep 2020 10:58:03	S	Std
10.0 - 1	510	35834	-	10.0000	7470A	PPB	11 Sep 2020 11:00:20	S	Std
ICV08 - 1	ICV08	13225	3.7006	-	7470A	PPB	11 Sep 2020 11:03:02	U	SMPL
ICB08 - 1	ICB08	-247	-0.0255	-	7470A	PPB	11 Sep 2020 11:05:17	U	SMPL
CCV89 - 1	CCV89	18502	5.1601	-	7470A	PPB	11 Sep 2020 11:07:32	U	SMPL
CCB89 - 1	CCB89	-242	-0.0241	-	7470A	PPB	11 Sep 2020 11:09:47	U	SMPL
CRA - 1	CRA	593	0.2069	-	7470A	PPB	11 Sep 2020 11:12:03	U	SMPL
HighStd - 1	HighStd	35675	9.9098	-	7470A	PPB	11 Sep 2020 11:14:18	U	SMPL
ChkStd - 1	ChkStd	24026	6.6879	-	7470A	PPB	11 Sep 2020 11:16:33	U	SMPL
PB131528BL - 1	PBW	-336	-0.0501	-	7470A	PPB	11 Sep 2020 11:18:50	U	SMPL
PB131528BS - 1	LCSW	13401	3.7493	-	7470A	PPB	11 Sep 2020 11:21:08	U	SMPL
L3941-04 - 1	RBR-200031	-195	-0.0111	-	7470A	PPB	11 Sep 2020 11:23:25	U	SMPL
L3941-04DUP - 1	RBR-200031DUP	-49	0.0293	-	7470A	PPB	11 Sep 2020 11:25:42	U	SMPL
L3941-04MS - 1	RBR-200031MS	13554	3.7916	-	7470A	PPB	11 Sep 2020 11:27:59	U	SMPL
L3941-04MSD - 1	RBR-200031MSD	14416	4.0300	-	7470A	PPB	11 Sep 2020 11:30:16	U	SMPL
L3942-02 - 1	N35868	-204	-0.0136	-	7470A	PPB	11 Sep 2020 11:32:32	U	SMPL
CCV90 - 1	CCV90	18345	5.1167	-	7470A	PPB	11 Sep 2020 11:34:48	U	SMPL
CCB90 - 1	CCB90	-231	-0.0211	-	7470A	PPB	11 Sep 2020 11:37:03	U	SMPL
PB131529BL - 1	PBW	-94	0.0168	-	7470A	PPB	11 Sep 2020 11:39:19	U	SMPL
PB131529BS - 1	LCSW	13684	3.8275	-	7470A	PPB	11 Sep 2020 11:41:34	U	SMPL
L3941-03 - 1	RBR-200031	4419	1.2650	-	7470A	PPB	11 Sep 2020 11:43:50	U	SMPL
L3942-01 - 1	N35868	5028	1.4335	-	7470A	PPB	11 Sep 2020 11:48:43	U	SMPL
L3942-01DUP - 1	N35868DUP	4779	1.3646	-	7470A	PPB	11 Sep 2020 11:53:44	U	SMPL
L3942-01MS - 1	N35868MS	18788	5.2392	-	7470A	PPB	11 Sep 2020 11:56:00	U	SMPL
L3942-01MSD - 1	N35868MSD	19568	5.4549	-	7470A	PPB	11 Sep 2020 11:58:16	U	SMPL
CCV91 - 1	CCV91	17426	4.8625	-	7470A	PPB	11 Sep 2020 12:00:34	U	SMPL
CCB91 - 1	CCB91	-137	0.0049	-	7470A	PPB	11 Sep 2020 12:02:51	U	SMPL
PB131528TB - 1	PB131510TB	-41	0.0315	-	7470A	PPB	11 Sep 2020 12:05:07	U	SMPL
L3941-04LX5 - 1		-31	0.0343	-	7470A	PPB	11 Sep 2020 12:07:23	U	SMPL
L3941-04A - 1		13067	3.6569	-	7470A	PPB	11 Sep 2020 12:09:39	U	SMPL
L3942-01LX5 - 1		702	0.2370	-	7470A	PPB	11 Sep 2020 12:11:54	U	SMPL
L3942-01A - 1		19470	5.4278	-	7470A	PPB	11 Sep 2020 12:14:10	U	SMPL
CCV92 - 1	CCV92	17306	4.8293	-	7470A	PPB	11 Sep 2020 12:16:25	U	SMPL
CCB92 - 1	CCB92	-183	-0.0078	-	7470A	PPB	11 Sep 2020 12:18:42	U	SMPL