


LB110916

245.1

INSTRUMENT ID: CY1

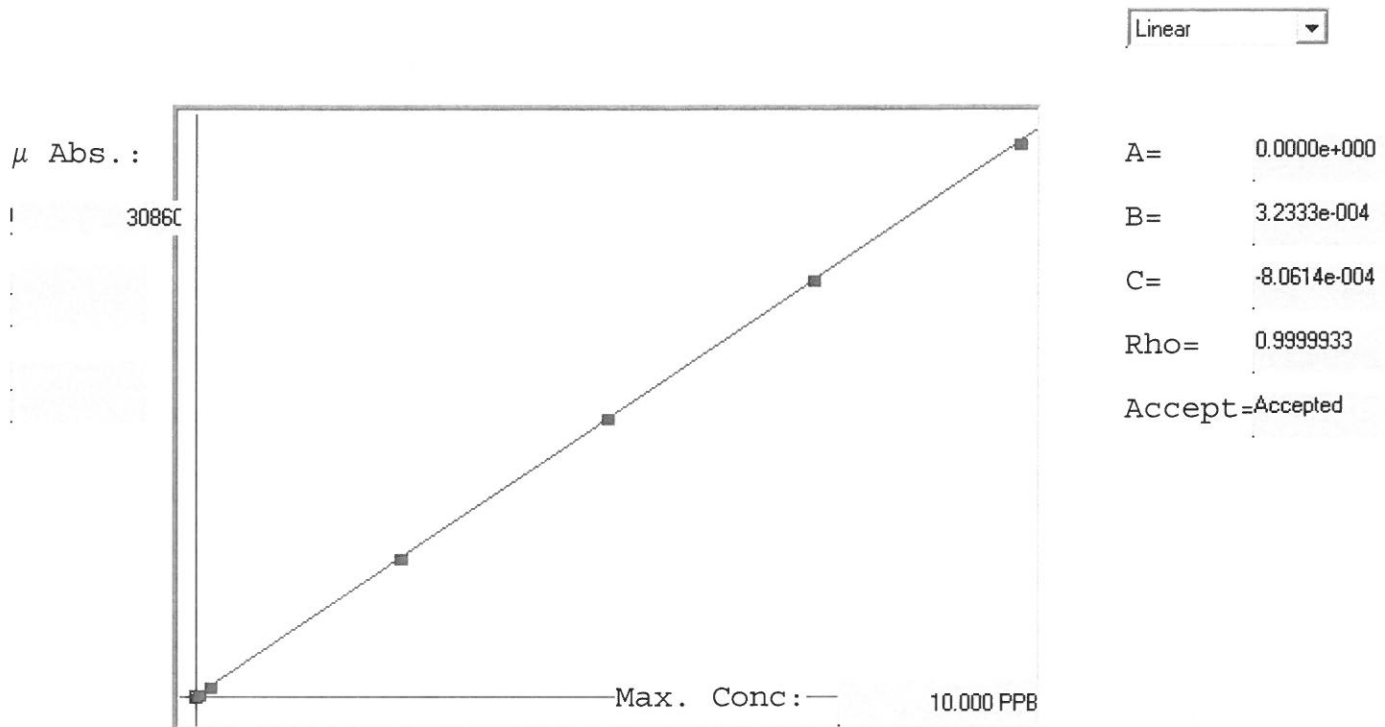

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.012	-0.012	-34	0.000	-34				
0.05	0.050	0.050	0.000	158	0.0 %	158				
0.2	0.200	0.197	-0.003	613	0.0 %	613				
2.5	2.500	2.502	0.002	7741	0.0 %	7741				
5.0	5.000	5.016	0.016	15515	0.0 %	15515				
7.5	7.500	7.519	0.019	23258	0.0 %	23258				
10.0	10.000	9.977	-0.023	30860	0.0 %	30860				

LB110916 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 11 Sep 2020 12:59:06

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-34	-	0.0000	245.1	PPB	11 Sep 2020 13:27:58	S	Std
0.05 - 1	50.05	158	-	0.0500	245.1	PPB	11 Sep 2020 13:30:16	S	Std
0.2 - 1	50.2	613	-	0.2000	245.1	PPB	11 Sep 2020 13:32:33	S	Std
2.5 - 1	52.5	7741	-	2.5000	245.1	PPB	11 Sep 2020 13:34:50	S	Std
5.0 - 1	55	15515	-	5.0000	245.1	PPB	11 Sep 2020 13:37:06	S	Std
7.5 - 1	57.5	23258	-	7.5000	245.1	PPB	11 Sep 2020 13:39:23	S	Std
10.0 - 1	511	30860	-	10.0000	245.1	PPB	11 Sep 2020 13:44:13	S	Std
ICV09 - 1	ICV09	12060	3.8986	-245.1		PPB	11 Sep 2020 13:54:33	U	SMPL
ICB09 - 1	ICB09	-66	-0.0221	-245.1		PPB	11 Sep 2020 13:56:48	U	SMPL
CCV93 - 1	CCV93	15088	4.8776	-245.1		PPB	11 Sep 2020 13:59:04	U	SMPL
CCB93 - 1	CCB93	-96	-0.0318	-245.1		PPB	11 Sep 2020 14:01:19	U	SMPL
CRA - 1	CRA	145	0.0461	-245.1		PPB	11 Sep 2020 14:06:07	U	SMPL
HighStd - 1	HighStd	29915	9.6716	-245.1		PPB	11 Sep 2020 14:08:22	U	SMPL
ChkStd - 1	ChkStd	20094	6.4962	-245.1		PPB	11 Sep 2020 14:10:38	U	SMPL
PB131551BL - 1	PBW	-49	-0.0166	-245.1		PPB	11 Sep 2020 14:15:32	U	SMPL
PB131551BS - 1	LCSW	11129	3.5975	-245.1		PPB	11 Sep 2020 14:17:47	U	SMPL
L3958-01 - 1	15220012-1	-174	-0.0571	-245.1		PPB	11 Sep 2020 14:20:03	U	SMPL
L3965-01 - 1	32220008-3	-156	-0.0512	-245.1		PPB	11 Sep 2020 14:22:21	U	SMPL
L3977-01 - 1	EFF-WW	50	0.0154	-245.1		PPB	11 Sep 2020 14:24:37	U	SMPL
L3977-01DUP - 1	EFF-WWDUP	17	0.0047	-245.1		PPB	11 Sep 2020 14:26:54	U	SMPL
L3977-01MS - 1	EFF-WWMS	9978	3.2254	-245.1		PPB	11 Sep 2020 14:29:09	U	SMPL
CCV94 - 1	CCV94	14885	4.8120	-245.1		PPB	11 Sep 2020 14:31:25	U	SMPL
CCB94 - 1	CCB94	-102	-0.0338	-245.1		PPB	11 Sep 2020 14:33:41	U	SMPL
L3977-01MSD - 1	EFF-WWMSD	10678	3.4517	-245.1		PPB	11 Sep 2020 14:39:31	U	SMPL
L3977-01LX5 - 1		-158	-0.0519	-245.1		PPB	11 Sep 2020 14:41:46	U	SMPL
L3977-01A - 1		12160	3.9309	-245.1		PPB	11 Sep 2020 14:44:02	U	SMPL
CCV95 - 1	CCV95	14575	4.7117	-245.1		PPB	11 Sep 2020 14:46:18	U	SMPL
CCB95 - 1	CCB95	-85	-0.0283	-245.1		PPB	11 Sep 2020 14:48:34	U	SMPL