


LB110976

7471B

INSTRUMENT ID: CY1

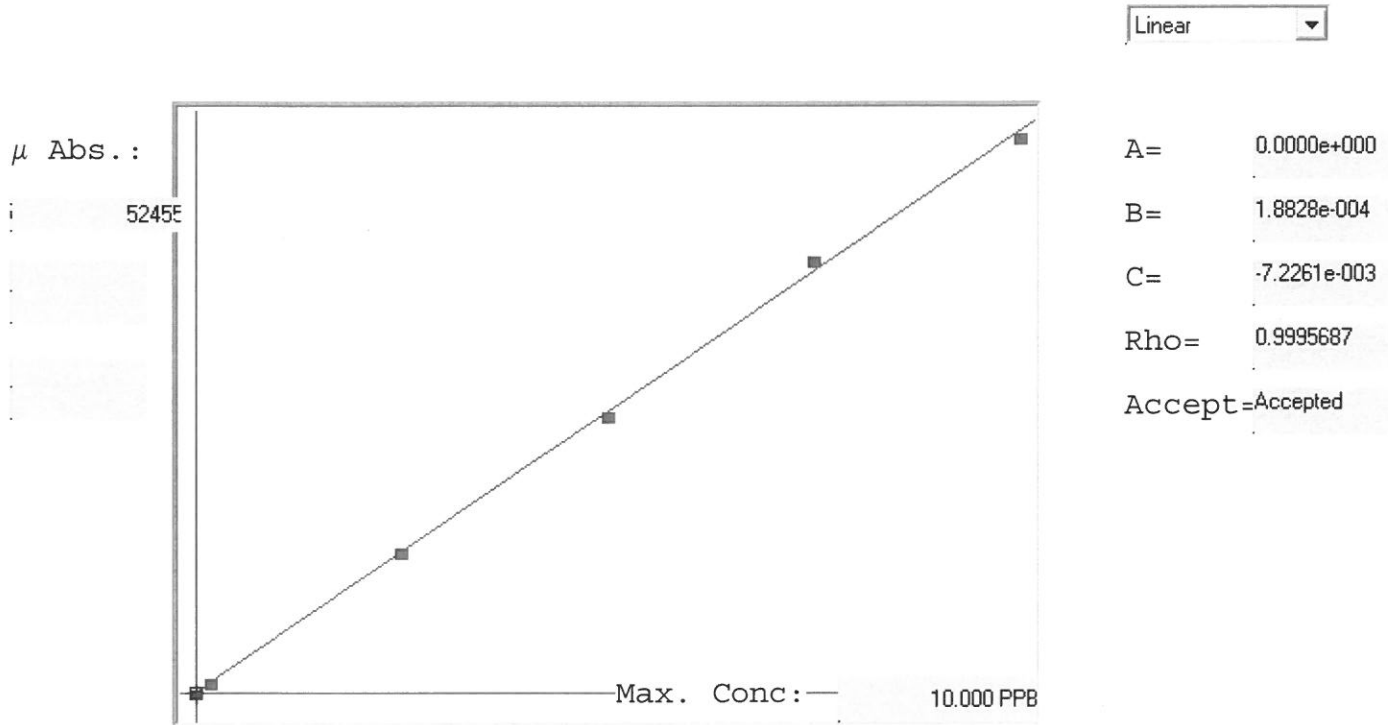

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.003	-0.003	22	0.000	22				
0.2	0.200	0.187	-0.013	1033	0.0 %	1033				
2.5	2.500	2.513	0.013	13383	0.0 %	13383				
5.0	5.000	4.919	-0.081	26162	0.0 %	26162				
7.5	7.500	7.715	0.215	41016	0.0 %	41016				
10.0	10.000	9.869	-0.131	52455	0.0 %	52455				

LB110976 INSTRUMENT ID : CV1

Method: 7471B		Operator: Admin		Date of Analysis: 15 Sep 2020 14:23:21					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S0	22	-	0.0000	7471B	PPB	15 Sep 2020 14:24:34	S	Std
0.2 - 1	S0.2	1033	-	0.2000	7471B	PPB	15 Sep 2020 14:26:51	S	Std
2.5 - 1	S2.5	13383	-	2.5000	7471B	PPB	15 Sep 2020 14:29:08	S	Std
5.0 - 1	S5	26162	-	5.0000	7471B	PPB	15 Sep 2020 14:31:25	S	Std
7.5 - 1	S7.5	41016	-	7.5000	7471B	PPB	15 Sep 2020 14:33:41	S	Std
10.0 - 1	S10	52455	-	10.0000	7471B	PPB	15 Sep 2020 14:35:58	S	Std
ICV14 - 1	ICV14	21718	4.0819	-	7471B	PPB	15 Sep 2020 14:38:49	U	SMPL
ICB14 - 1	ICB14	-120	-0.0298	-	7471B	PPB	15 Sep 2020 14:41:04	U	SMPL
CCV16 - 1	CCV16	26459	4.9746	-	7471B	PPB	15 Sep 2020 14:43:20	U	SMPL
CCB16 - 1	CCB16	-130	-0.0317	-	7471B	PPB	15 Sep 2020 14:45:36	U	SMPL
CRA - 1	CRA	998	0.1807	-	7471B	PPB	15 Sep 2020 14:47:52	U	SMPL
HighStd - 1	HighStd	52443	9.8669	-	7471B	PPB	15 Sep 2020 14:50:07	U	SMPL
ChkStd - 1	ChkStd	36968	6.9532	-	7471B	PPB	15 Sep 2020 14:52:22	U	SMPL
PB131625BL - 1	PBS	-148	-0.0351	-	7471B	PPB	15 Sep 2020 14:54:39	U	SMPL
PB131625BS - 1	LCSS	19417	3.6487	-	7471B	PPB	15 Sep 2020 14:56:57	U	SMPL
L3867-01 - 1	EO-02-091420	4686	0.8751	-	7471B	PPB	15 Sep 2020 14:59:13	U	SMPL
L3871-07 - 1	TR-04-091420	3622	0.6747	-	7471B	PPB	15 Sep 2020 15:01:30	U	SMPL
L3998-01 - 1	FK-EF-01-TEST1-ABCD-A	2882	0.5354	-	7471B	PPB	15 Sep 2020 15:03:47	U	SMPL
L3998-03 - 1	FK-EF-01-TEST1-ABCD-B	2255	0.4174	-	7471B	PPB	15 Sep 2020 15:06:05	U	SMPL
L4005-01 - 1	22-31	24989	4.6978	-	7471B	PPB	15 Sep 2020 15:08:20	U	SMPL
CCV17 - 1	CCV17	26650	5.0105	-	7471B	PPB	15 Sep 2020 15:10:35	U	SMPL
CCB17 - 1	CCB17	-98	-0.0257	-	7471B	PPB	15 Sep 2020 15:12:52	U	SMPL
L4005-03 - 1	32-34	23169	4.3551	-	7471B	PPB	15 Sep 2020 15:15:07	U	SMPL
L4007-01 - 1	72-11929	1521	0.2792	-	7471B	PPB	15 Sep 2020 15:17:22	U	SMPL
L4008-01 - 1	40951	795	0.1425	-	7471B	PPB	15 Sep 2020 15:19:38	U	SMPL
L4009-01 - 1	HAYES-SEYMOUR-01	4944	0.9236	-	7471B	PPB	15 Sep 2020 15:21:54	U	SMPL
L4013-03 - 1	PAV-B40-091420-0-10	23893	4.4914	-	7471B	PPB	15 Sep 2020 15:36:48	U	SMPL
L4013-03DUP - 1	PAV-B40-091420-0-10DUP	24474	4.6008	-	7471B	PPB	15 Sep 2020 15:39:04	U	SMPL
L4013-03MS - 1	PAV-B40-091420-0-10MS	45139	8.4917	-	7471B	PPB	15 Sep 2020 15:41:21	U	SMPL
L4013-03MSD - 1	PAV-B40-091420-0-10MSD	45139	8.4917	-	7471B	PPB	15 Sep 2020 15:43:39	U	SMPL
L4013-05 - 1	PAV-B40-091420-10-15	12518	2.3497	-	7471B	PPB	15 Sep 2020 15:45:58	U	SMPL
CCV18 - 1	CCV18	26751	5.0295	-	7471B	PPB	15 Sep 2020 15:48:15	U	SMPL
CCB18 - 1	CCB18	-116	-0.0291	-	7471B	PPB	15 Sep 2020 15:50:32	U	SMPL
L4013-03LX5 - 1		4827	0.9016	-	7471B	PPB	15 Sep 2020 15:52:48	U	SMPL
L4013-03A - 1		45021	8.4695	-	7471B	PPB	15 Sep 2020 15:55:04	U	SMPL
CCV19 - 1	CCV19	26580	4.9973	-	7471B	PPB	15 Sep 2020 15:58:57	U	SMPL
CCB19 - 1	CCB19	-122	-0.0302	-	7471B	PPB	15 Sep 2020 16:01:12	U	SMPL