


LB110988

7470A

INSTRUMENT ID: CY1

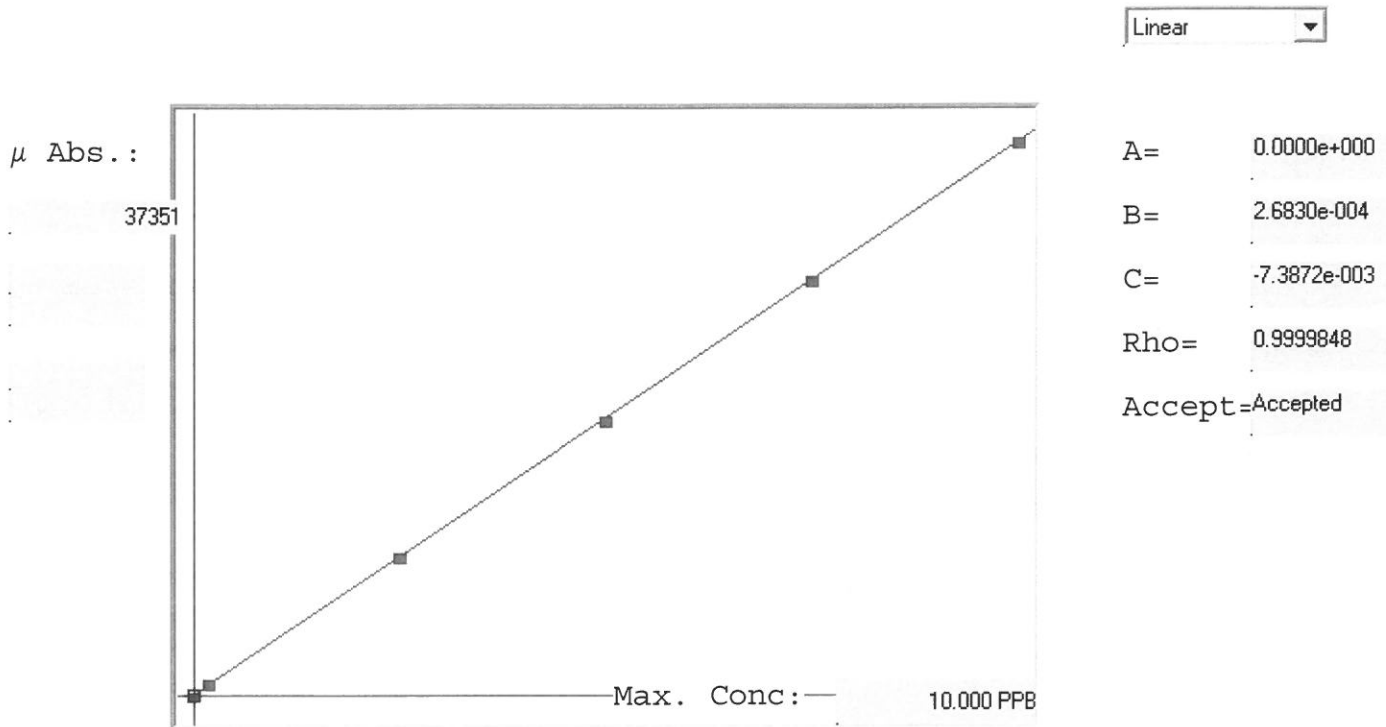

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.011	-0.011	-15	0.000	-15				
0.2	0.200	0.223	0.023	857	0.0 %	857				
2.5	2.500	2.511	0.011	9387	0.0 %	9387				
5.0	5.000	4.961	-0.039	18518	0.0 %	18518				
7.5	7.500	7.503	0.003	27992	0.0 %	27992				
10.0	10.000	10.014	0.014	37351	0.0 %	37351				

LB110988 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 16 Sep 2020 09:31:16

Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	-15	-	0.00007470A	PPB	16 Sep 2020 09:32:55	S	Std
0.2 - 1	50.2	857	-	0.20007470A	PPB	16 Sep 2020 09:35:13	S	Std
2.5 - 1	52.5	9387	-	2.50007470A	PPB	16 Sep 2020 09:37:30	S	Std
5.0 - 1	55	18518	-	5.00007470A	PPB	16 Sep 2020 09:39:47	S	Std
7.5 - 1	57.5	27992	-	7.50007470A	PPB	16 Sep 2020 09:42:03	S	Std
10.0 - 1	511	37351	-	10.00007470A	PPB	16 Sep 2020 09:44:19	S	Std
ICV15 - 1	ICV15	13960	3.7381	-7470A	PPB	16 Sep 2020 09:47:08	U	SMPL
ICB15 - 1	ICB15	-290	-0.0852	-7470A	PPB	16 Sep 2020 09:49:23	U	SMPL
CCV20 - 1	CCV20	18143	4.8604	-7470A	PPB	16 Sep 2020 09:51:38	U	SMPL
CCB20 - 1	CCB20	-260	-0.0771	-7470A	PPB	16 Sep 2020 09:53:53	U	SMPL
CRA - 1	CRA	873	0.2268	-7470A	PPB	16 Sep 2020 09:56:09	U	SMPL
HighStd - 1	HighStd	35306	9.4652	-7470A	PPB	16 Sep 2020 09:58:24	U	SMPL
ChkStd - 1	ChkStd	23477	6.2915	-7470A	PPB	16 Sep 2020 10:00:39	U	SMPL
PB131634BL - 1	PBW	170	0.0382	-7470A	PPB	16 Sep 2020 10:02:57	U	SMPL
PB131634BS - 1	LCSW	14124	3.7821	-7470A	PPB	16 Sep 2020 10:05:14	U	SMPL
L3979-04 - 1	40-42	156	0.0345	-7470A	PPB	16 Sep 2020 10:07:31	U	SMPL
L3979-04DUP - 1	40-42DUP	145	0.0315	-7470A	PPB	16 Sep 2020 10:13:41	U	SMPL
L3979-04MS - 1	40-42MS	13395	3.5865	-7470A	PPB	16 Sep 2020 10:18:36	U	SMPL
L3979-04MSD - 1	40-42MSD	13937	3.7319	-7470A	PPB	16 Sep 2020 10:20:53	U	SMPL
L3980-01 - 1	31239	716	0.1847	-7470A	PPB	16 Sep 2020 10:23:09	U	SMPL
CCV21 - 1	CCV21	18041	4.8330	-7470A	PPB	16 Sep 2020 10:25:24	U	SMPL
CCB21 - 1	CCB21	-245	-0.0731	-7470A	PPB	16 Sep 2020 10:27:40	U	SMPL
PB131635BL - 1	PBW	317	0.0777	-7470A	PPB	16 Sep 2020 10:29:56	U	SMPL
PB131635BS - 1	LCSW	13480	3.6093	-7470A	PPB	16 Sep 2020 10:32:11	U	SMPL
L3867-06 - 1	EO-02-091420	310	0.0758	-7470A	PPB	16 Sep 2020 10:34:27	U	SMPL
L3867-06DUP - 1	EO-02-091420DUP	386	0.0962	-7470A	PPB	16 Sep 2020 10:45:33	U	SMPL
L3867-06MS - 1	EO-02-091420MS	14893	3.9884	-7470A	PPB	16 Sep 2020 10:47:49	U	SMPL
L3867-06MSD - 1	EO-02-091420MSD	14104	3.7767	-7470A	PPB	16 Sep 2020 10:50:05	U	SMPL
L3871-10 - 1	TR-04-091420	638	0.1638	-7470A	PPB	16 Sep 2020 10:52:22	U	SMPL
L4005-02 - 1	22-31	576	0.1472	-7470A	PPB	16 Sep 2020 10:54:39	U	SMPL
L4005-04 - 1	32-34	212	0.0495	-7470A	PPB	16 Sep 2020 10:56:57	U	SMPL
L4005-05 - 1	35-37	308	0.0752	-7470A	PPB	16 Sep 2020 10:59:12	U	SMPL
CCV22 - 1	CCV22	18007	4.8239	-7470A	PPB	16 Sep 2020 11:01:28	U	SMPL
CCB22 - 1	CCB22	143	0.0310	-7470A	PPB	16 Sep 2020 11:03:43	U	SMPL
L4007-02 - 1	72-11929	205	0.0476	-7470A	PPB	16 Sep 2020 11:05:59	U	SMPL
L4013-04 - 1	PAV-B40-091420-0-10	241	0.0573	-7470A	PPB	16 Sep 2020 11:08:15	U	SMPL
L4013-06 - 1	PAV-B40-091420-10-15	206	0.0479	-7470A	PPB	16 Sep 2020 11:10:30	U	SMPL
PB131636BL - 1	PBW	183	0.0417	-7470A	PPB	16 Sep 2020 11:12:46	U	SMPL
PB131636BS - 1	LCSW	13697	3.6675	-7470A	PPB	16 Sep 2020 11:15:02	U	SMPL
L4009-02 - 1	HAYES-SEYMOUR-01	755	0.1952	-7470A	PPB	16 Sep 2020 11:22:11	U	SMPL
L4009-02DUP - 1	HAYES-SEYMOUR-01DUP	714	0.1842	-7470A	PPB	16 Sep 2020 11:27:07	U	SMPL
L4009-02MS - 1	HAYES-SEYMOUR-01MS	14262	3.8191	-7470A	PPB	16 Sep 2020 11:29:24	U	SMPL
L4009-02MSD - 1	HAYES-SEYMOUR-01MSD	15445	4.1365	-7470A	PPB	16 Sep 2020 11:31:41	U	SMPL
CCV23 - 1	CCV23	18186	4.8719	-7470A	PPB	16 Sep 2020 11:33:57	U	SMPL
CCB23 - 1	CCB23	-86	-0.0305	-7470A	PPB	16 Sep 2020 11:36:13	U	SMPL
PB131634TB - 1	PB131570TB	241	0.0573	-7470A	PPB	16 Sep 2020 11:41:03	U	SMPL
PB131635TB - 1	PB131606TB	131	0.0278	-7470A	PPB	16 Sep 2020 11:43:18	U	SMPL
PB131636TB - 1	PB131605TB	155	0.0342	-7470A	PPB	16 Sep 2020 11:45:34	U	SMPL
L3979-04LX5 - 1		89	0.0165	-7470A	PPB	16 Sep 2020 11:47:49	U	SMPL
L3979-04A - 1		14004	3.7499	-7470A	PPB	16 Sep 2020 11:50:05	U	SMPL
L3867-06LX5 - 1		26	-0.0004	-7470A	PPB	16 Sep 2020 11:52:21	U	SMPL
L3867-06A - 1		14925	3.9970	-7470A	PPB	16 Sep 2020 11:54:37	U	SMPL
L4009-02LX5 - 1		376	0.0935	-7470A	PPB	16 Sep 2020 11:56:53	U	SMPL
L4009-02A - 1		15663	4.1950	-7470A	PPB	16 Sep 2020 11:59:10	U	SMPL
CCV24 - 1	CCV24	18148	4.8617	-7470A	PPB	16 Sep 2020 12:01:26	U	SMPL
CCB24 - 1	CCB24	25	-0.0007	-7470A	PPB	16 Sep 2020 12:03:43	U	SMPL