


LB 110992

7471B

INSTRUMENT ID: CV4

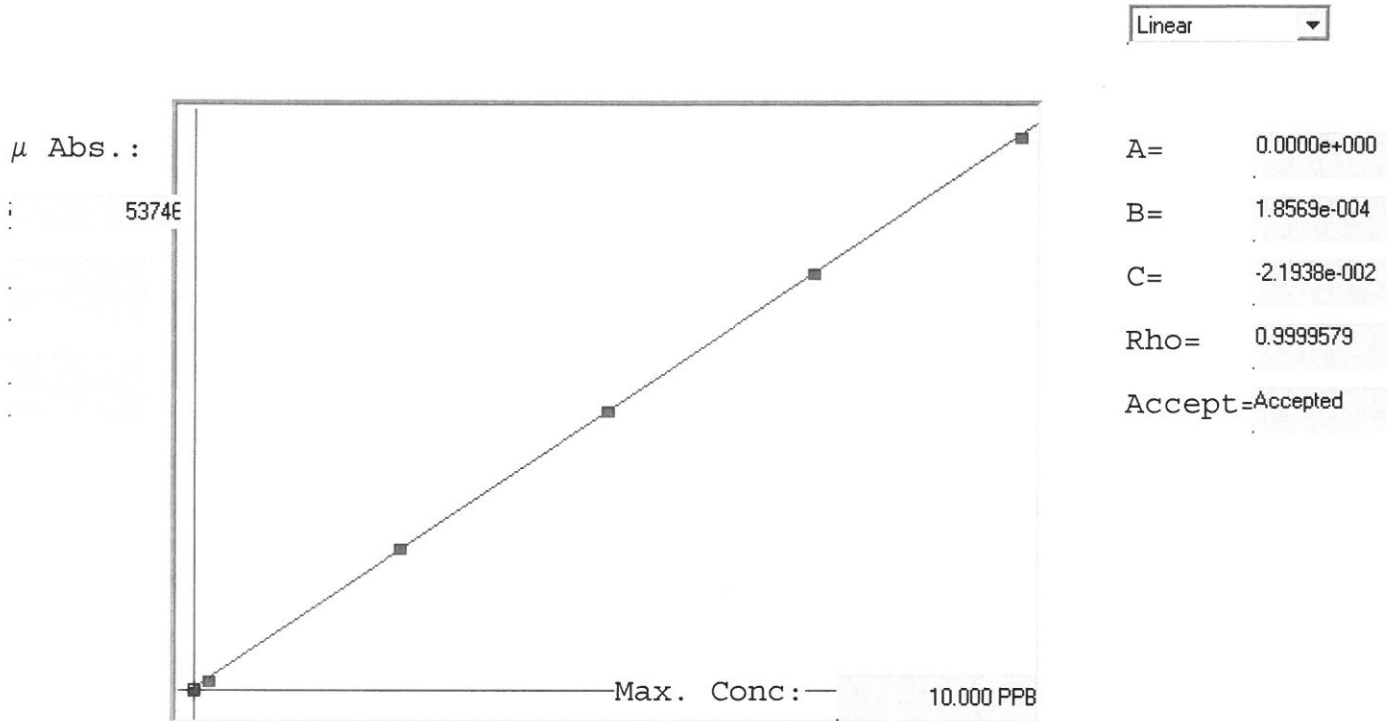

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.015	-0.015	35	0.000	35				
0.2	0.200	0.162	-0.038	992	0.0 %	992				
2.5	2.500	2.537	0.037	13782	0.0 %	13782				
5.0	5.000	5.043	0.043	27276	0.0 %	27276				
7.5	7.500	7.515	0.015	40591	0.0 %	40591				
10.0	10.000	9.958	-0.042	53746	0.0 %	53746				

LB110992 INSTRUMENT ID : CV1

Method: 7471B	Operator: Admin	Date of Analysis: 16 Sep 2020 12:18:57						
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	S0	35	-	0.00007471B	PPB	16 Sep 2020 12:19:48	S	Std
0.2 - 1	S0.2	992	-	0.20007471B	PPB	16 Sep 2020 12:22:05	S	Std
2.5 - 1	S2.5	13782	-	2.50007471B	PPB	16 Sep 2020 12:24:23	S	Std
5.0 - 1	S5	27276	-	5.00007471B	PPB	16 Sep 2020 12:26:40	S	Std
7.5 - 1	S7.5	40591	-	7.50007471B	PPB	16 Sep 2020 12:28:56	S	Std
10.0 - 1	S10	53746	-	10.00007471B	PPB	16 Sep 2020 12:31:12	S	Std
ICV16 - 1	ICV16	21432	3.9577	-7471B	PPB	16 Sep 2020 12:34:00	U	SMPL
ICB16 - 1	ICB16	-105	-0.0414	-7471B	PPB	16 Sep 2020 12:36:15	U	SMPL
CCV25 - 1	CCV25	27356	5.0577	-7471B	PPB	16 Sep 2020 12:38:31	U	SMPL
CCB25 - 1	CCB25	-92	-0.0390	-7471B	PPB	16 Sep 2020 12:40:46	U	SMPL
CRA - 1	CRA	969	0.1580	-7471B	PPB	16 Sep 2020 12:43:02	U	SMPL
HighStd - 1	HighStd	54163	10.0354	-7471B	PPB	16 Sep 2020 12:45:18	U	SMPL
ChkStd - 1	ChkStd	36617	6.7773	-7471B	PPB	16 Sep 2020 12:48:49	U	SMPL
PB131648BL - 1	PBS	-254	-0.0691	-7471B	PPB	16 Sep 2020 12:51:04	U	SMPL
PB131648BS - 1	LCSS	21105	3.8970	-7471B	PPB	16 Sep 2020 12:53:22	U	SMPL
L3868-01 - 1	PL-02-091520	3692	0.6636	-7471B	PPB	16 Sep 2020 12:55:38	U	SMPL
L4015-01 - 1	REACTOR-6E-(A-D-0-4)	34872	6.4533	-7471B	PPB	16 Sep 2020 12:57:55	U	SMPL
L4015-12 - 1	REACTOR-5W-(A-D-0-4)	19624	3.6220	-7471B	PPB	16 Sep 2020 13:00:12	U	SMPL
L4018-01 - 1	LACY-08	3539	0.6352	-7471B	PPB	16 Sep 2020 13:02:30	U	SMPL
L4018-04 - 1	VNJ-229	922	0.1493	-7471B	PPB	16 Sep 2020 13:04:46	U	SMPL
CCV26 - 1	CCV26	27468	5.0785	-7471B	PPB	16 Sep 2020 13:07:01	U	SMPL
CCB26 - 1	CCB26	-99	-0.0403	-7471B	PPB	16 Sep 2020 13:09:16	U	SMPL
L4019-01 - 1	VNJ-220	3342	0.5986	-7471B	PPB	16 Sep 2020 13:11:32	U	SMPL
L4020-01 - 1	ETGI-362	4996	0.9057	-7471B	PPB	16 Sep 2020 13:13:48	U	SMPL
L4020-03 - 1	ETGI-370	3203	0.5728	-7471B	PPB	16 Sep 2020 13:16:03	U	SMPL
L4020-03DUP - 1	ETGI-370DUP	3578	0.6424	-7471B	PPB	16 Sep 2020 13:18:19	U	SMPL
L4020-03MS - 1	ETGI-370MS	23204	4.2867	-7471B	PPB	16 Sep 2020 13:20:35	U	SMPL
L4020-03MSD - 1	ETGI-370MSD	23259	4.2969	-7471B	PPB	16 Sep 2020 13:22:52	U	SMPL
L4021-01 - 1	B14-1-3	3751	0.6746	-7471B	PPB	16 Sep 2020 13:25:08	U	SMPL
L4021-02 - 1	B14-5-7	11845	2.1775	-7471B	PPB	16 Sep 2020 13:27:25	U	SMPL
L4021-03 - 1	B15-1-3	6176	1.1249	-7471B	PPB	16 Sep 2020 13:29:43	U	SMPL
L4021-04 - 1	B15-5-7	9457	1.7341	-7471B	PPB	16 Sep 2020 13:31:59	U	SMPL
CCV27 - 1	CCV27	27564	5.0963	-7471B	PPB	16 Sep 2020 13:34:15	U	SMPL
CCB27 - 1	CCB27	-78	-0.0364	-7471B	PPB	16 Sep 2020 13:36:30	U	SMPL
L4021-05 - 1	B15A-5-7	13764	2.5338	-7471B	PPB	16 Sep 2020 13:38:46	U	SMPL
L4021-06 - 1	B16-1-3	4200	0.7579	-7471B	PPB	16 Sep 2020 13:41:01	U	SMPL
L4021-07 - 1	B16-5-7	9041	1.6568	-7471B	PPB	16 Sep 2020 13:43:17	U	SMPL
L4029-01 - 1	WC-PM-B2-0-3.5-C	2217	0.3897	-7471B	PPB	16 Sep 2020 13:45:32	U	SMPL
L4020-03LX5 - 1		555	0.0811	-7471B	PPB	16 Sep 2020 13:47:48	U	SMPL
L4020-03A - 1		23005	4.2498	-7471B	PPB	16 Sep 2020 13:50:04	U	SMPL
CCV28 - 1	CCV28	27280	5.0436	-7471B	PPB	16 Sep 2020 13:52:21	U	SMPL
CCB28 - 1	CCB28	-45	-0.0303	-7471B	PPB	16 Sep 2020 13:54:37	U	SMPL