


LB111012

7470A

INSTRUMENT ID: CV1

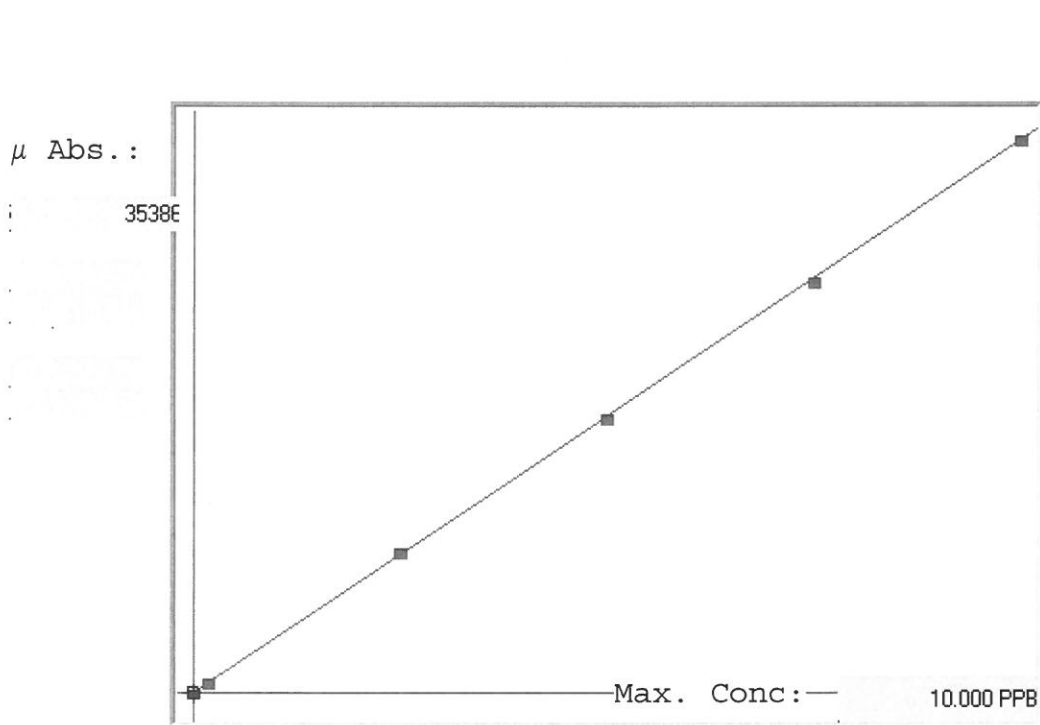

Linear

A= 0.0000e+000

B= 2.8317e-004

C= 4.1132e-003

Rho= 0.9999674

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	-22	0.000	-22				
0.2	0.200	0.182	-0.018	627	0.0 %	627				
2.5	2.500	2.551	0.051	8994	0.0 %	8994				
5.0	5.000	4.985	-0.015	17588	0.0 %	17588				
7.5	7.500	7.461	-0.039	26332	0.0 %	26332				
10.0	10.000	10.024	0.024	35386	0.0 %	35386				

LB111012 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 17 Sep 2020 09:30:04					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-22	-	0.0000	7470A	PPB	17 Sep 2020 09:32:01	S	Std
0.2 - 1	50.2	627	-	0.2000	7470A	PPB	17 Sep 2020 09:34:18	S	Std
2.5 - 1	52.5	8994	-	2.5000	7470A	PPB	17 Sep 2020 09:36:36	S	Std
5.0 - 1	55	17588	-	5.0000	7470A	PPB	17 Sep 2020 09:38:53	S	Std
7.5 - 1	57.5	26332	-	7.5000	7470A	PPB	17 Sep 2020 09:41:11	S	Std
10.0 - 1	510	35386	-	10.0000	7470A	PPB	17 Sep 2020 09:46:03	S	Std
ICV17 - 1	ICV17	13190	3.7391	-	7470A	PPB	17 Sep 2020 09:48:43	U	SMPL
ICB17 - 1	ICB17	-176	-0.0457	-	7470A	PPB	17 Sep 2020 09:50:58	U	SMPL
CCV33 - 1	CCV33	18026	5.1086	-	7470A	PPB	17 Sep 2020 09:53:13	U	SMPL
CCB33 - 1	CCB33	-167	-0.0432	-	7470A	PPB	17 Sep 2020 09:55:29	U	SMPL
CRA - 1	CRA	593	0.1720	-	7470A	PPB	17 Sep 2020 09:57:45	U	SMPL
HighStd - 1	HighStd	35645	10.0977	-	7470A	PPB	17 Sep 2020 10:00:00	U	SMPL
ChkStd - 1	ChkStd	23638	6.6977	-	7470A	PPB	17 Sep 2020 10:02:16	U	SMPL
PB131667BL - 1	PBW	-279	-0.0749	-	7470A	PPB	17 Sep 2020 10:04:34	U	SMPL
PB131667BS - 1	LCSW	13760	3.9005	-	7470A	PPB	17 Sep 2020 10:06:51	U	SMPL
L3868-06 - 1	PL-02-091520	-31	-0.0047	-	7470A	PPB	17 Sep 2020 10:14:09	U	SMPL
L3868-06DUP - 1	PL-02-091520DUP	-24	-0.0027	-	7470A	PPB	17 Sep 2020 10:16:25	U	SMPL
L3868-06MS - 1	PL-02-091520MS	13664	3.8734	-	7470A	PPB	17 Sep 2020 10:18:42	U	SMPL
L3868-06MSD - 1	PL-02-091520MSD	12674	3.5930	-	7470A	PPB	17 Sep 2020 10:21:00	U	SMPL
L4015-02 - 1	REACTOR-6E-(A-D-0-4)	-150	-0.0384	-	7470A	PPB	17 Sep 2020 10:23:16	U	SMPL
CCV34 - 1	CCV34	18171	5.1496	-	7470A	PPB	17 Sep 2020 10:25:32	U	SMPL
CCB34 - 1	CCB34	-162	-0.0418	-	7470A	PPB	17 Sep 2020 10:27:47	U	SMPL
L4015-13 - 1	REACTOR-5W-(A-D-0-4)	-40	-0.0072	-	7470A	PPB	17 Sep 2020 10:30:03	U	SMPL
L4018-02 - 1	LACY-08	-21	-0.0018	-	7470A	PPB	17 Sep 2020 10:32:19	U	SMPL
L4018-05 - 1	VNJ-229	-19	-0.0013	-	7470A	PPB	17 Sep 2020 10:34:35	U	SMPL
L4019-02 - 1	VNJ-220	-12	0.0007	-	7470A	PPB	17 Sep 2020 10:36:50	U	SMPL
L4020-02 - 1	ETGI-362	-14	0.0001	-	7470A	PPB	17 Sep 2020 10:39:06	U	SMPL
L4020-04 - 1	ETGI-370	-3	0.0033	-	7470A	PPB	17 Sep 2020 10:41:23	U	SMPL
PB131668BL - 1	PBW	-6	0.0024	-	7470A	PPB	17 Sep 2020 10:43:40	U	SMPL
PB131668BS - 1	LCSW	13469	3.8181	-	7470A	PPB	17 Sep 2020 10:45:57	U	SMPL
L4008-02 - 1	13703	796	0.2295	-	7470A	PPB	17 Sep 2020 10:53:25	U	SMPL
CCV35 - 1	CCV35	18033	5.1105	-	7470A	PPB	17 Sep 2020 10:57:55	U	SMPL
CCB35 - 1	CCB35	-86	-0.0202	-	7470A	PPB	17 Sep 2020 11:00:11	U	SMPL
L4008-02MS - 1	13703MS	11542	3.2725	-	7470A	PPB	17 Sep 2020 11:02:27	U	SMPL
L4008-02MSD - 1	13703MSD	11246	3.1887	-	7470A	PPB	17 Sep 2020 11:04:42	U	SMPL
L4021-08 - 1	FIELD-BLANK	-191	-0.0500	-	7470A	PPB	17 Sep 2020 11:06:59	U	SMPL
L4038-13 - 1	FIELD-BLANK	0	0.0041	-	7470A	PPB	17 Sep 2020 11:09:16	U	SMPL
PB131667TB - 1	PB131645TB	-4	0.0030	-	7470A	PPB	17 Sep 2020 11:11:32	U	SMPL
L4008-02DUP - 1	13703DUP	691	0.1998	-	7470A	PPB	17 Sep 2020 11:13:49	U	SMPL
L3868-06LX5 - 1		-15	-0.0001	-	7470A	PPB	17 Sep 2020 11:16:05	U	SMPL
L3868-06A - 1		13652	3.8700	-	7470A	PPB	17 Sep 2020 11:18:22	U	SMPL
L4008-02LX5 - 1		302	0.0896	-	7470A	PPB	17 Sep 2020 11:20:40	U	SMPL
L4008-02A - 1		14012	3.9719	-	7470A	PPB	17 Sep 2020 11:22:55	U	SMPL
CCV36 - 1	CCV36	18229	5.1660	-	7470A	PPB	17 Sep 2020 11:25:11	U	SMPL
CCB36 - 1	CCB36	-101	-0.0245	-	7470A	PPB	17 Sep 2020 11:27:27	U	SMPL