


LB111034

7470A

INSTRUMENT ID: CV1

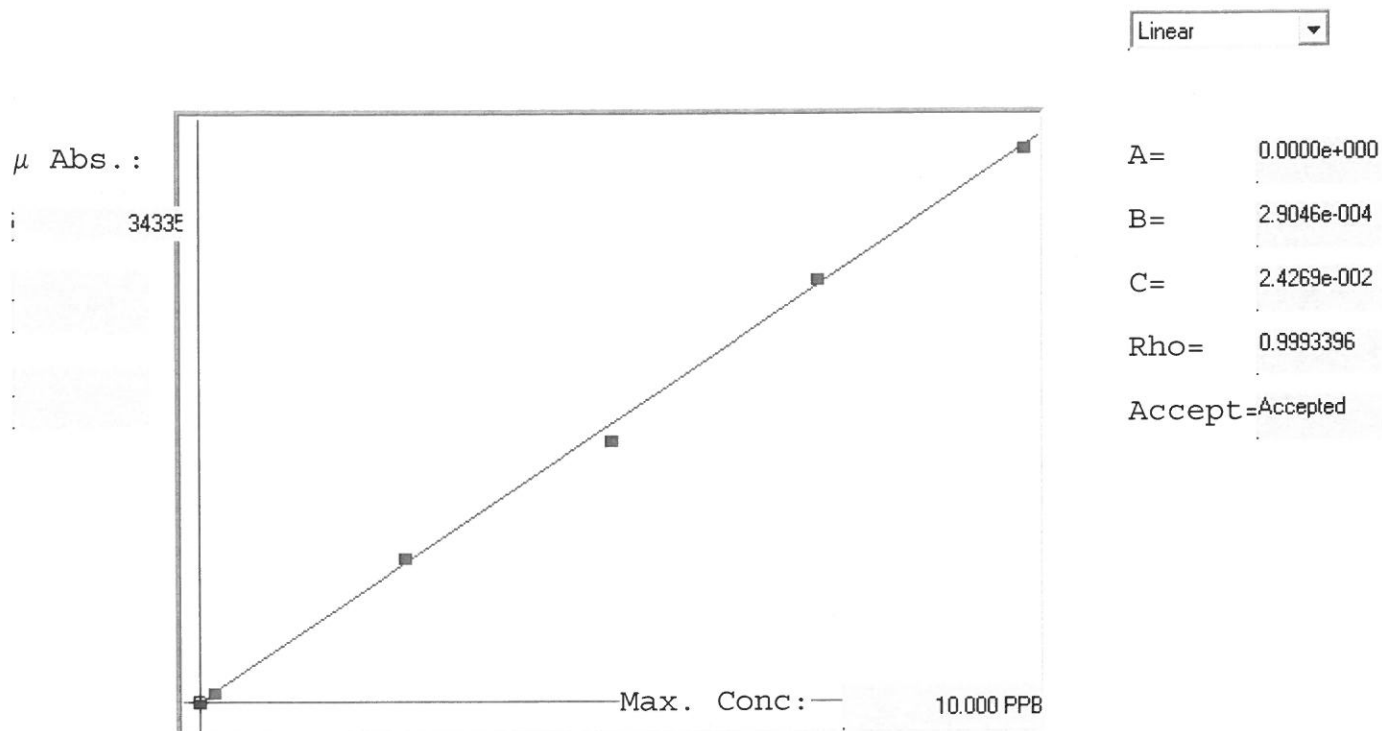

| Std ID | Conc.  | Calc. | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 |
|--------|--------|-------|--------|-------|------------|-------|-------|-------|-------|-------|
| 0.0    | 0.000  | 0.017 | 0.017  | -24   | 0.000      | -24   |       |       |       |       |
| 0.2    | 0.200  | 0.201 | 0.001  | 607   | 0.0 %      | 607   |       |       |       |       |
| 2.5    | 2.500  | 2.630 | 0.130  | 8970  | 0.0 %      | 8970  |       |       |       |       |
| 5.0    | 5.000  | 4.727 | -0.273 | 16192 | 0.0 %      | 16192 |       |       |       |       |
| 7.5    | 7.500  | 7.628 | 0.128  | 26179 | 0.0 %      | 26179 |       |       |       |       |
| 10.0   | 10.000 | 9.997 | -0.003 | 34335 | 0.0 %      | 34335 |       |       |       |       |

# LB111034 INSTRUMENT ID : CV1

| Method: 7470A   |                         | Operator: Admin |         | Date of Analysis: 18 Sep 2020 09:58:40 |        |       |                      |      |      |
|-----------------|-------------------------|-----------------|---------|----------------------------------------|--------|-------|----------------------|------|------|
| Sample ID       | Extended ID             | μ Abs.          | Conc.   | Std Conc                               | Method | Units | Date                 | Type | Type |
| 0.0 - 1         | 50                      | -24             | -       | 0.00007470A                            |        | PPB   | 18 Sep 2020 10:00:14 | S    | Std  |
| 0.2 - 1         | 50.2                    | 607             | -       | 0.20007470A                            |        | PPB   | 18 Sep 2020 10:02:31 | S    | Std  |
| 2.5 - 1         | 52.5                    | 8970            | -       | 2.50007470A                            |        | PPB   | 18 Sep 2020 10:04:48 | S    | Std  |
| 5.0 - 1         | 55                      | 16192           | -       | 5.00007470A                            |        | PPB   | 18 Sep 2020 10:07:05 | S    | Std  |
| 7.5 - 1         | 57.5                    | 26179           | -       | 7.50007470A                            |        | PPB   | 18 Sep 2020 10:09:21 | S    | Std  |
| 10.0 - 1        | 50                      | 34335           | -       | 10.00007470A                           |        | PPB   | 18 Sep 2020 10:11:38 | S    | Std  |
| ICV19 - 1       | ICV19                   | 13113           | 3.8330  | -7470A                                 |        | PPB   | 18 Sep 2020 10:14:23 | U    | SMPL |
| ICB19 - 1       | ICB19                   | -203            | -0.0347 | -7470A                                 |        | PPB   | 18 Sep 2020 10:16:37 | U    | SMPL |
| CCV42 - 1       | CCV42                   | 16880           | 4.9272  | -7470A                                 |        | PPB   | 18 Sep 2020 10:18:52 | U    | SMPL |
| CCB42 - 1       | CCB42                   | -225            | -0.0411 | -7470A                                 |        | PPB   | 18 Sep 2020 10:21:07 | U    | SMPL |
| CRA - 1         | CRA                     | 570             | 0.1898  | -7470A                                 |        | PPB   | 18 Sep 2020 10:23:23 | U    | SMPL |
| HighStd - 1     | HighStd                 | 34896           | 10.1600 | -7470A                                 |        | PPB   | 18 Sep 2020 10:25:38 | U    | SMPL |
| ChkStd - 1      | ChkStd                  | 24324           | 7.0893  | -7470A                                 |        | PPB   | 18 Sep 2020 10:27:55 | U    | SMPL |
| PB131699BL - 1  | PBW                     | -279            | -0.0568 | -7470A                                 |        | PPB   | 18 Sep 2020 10:30:13 | U    | SMPL |
| PB131699BS - 1  | LCSW                    | 13867           | 4.0520  | -7470A                                 |        | PPB   | 18 Sep 2020 10:32:30 | U    | SMPL |
| L4038-04 - 1    | PAV-B36-091620-0-10     | -160            | -0.0222 | -7470A                                 |        | PPB   | 18 Sep 2020 10:34:47 | U    | SMPL |
| L4038-08 - 1    | PAV-091620-DP           | -46             | 0.0109  | -7470A                                 |        | PPB   | 18 Sep 2020 10:37:04 | U    | SMPL |
| L4038-10 - 1    | PAV-B36-091620-10-15    | -30             | 0.0156  | -7470A                                 |        | PPB   | 18 Sep 2020 10:39:21 | U    | SMPL |
| L4038-10DUP - 1 | PAV-B36-091620-10-15DUP | -22             | 0.0179  | -7470A                                 |        | PPB   | 18 Sep 2020 10:41:38 | U    | SMPL |
| L4038-10MS - 1  | PAV-B36-091620-10-15MS  | 14329           | 4.1862  | -7470A                                 |        | PPB   | 18 Sep 2020 10:43:54 | U    | SMPL |
| CCV43 - 1       | CCV43                   | 17033           | 4.9716  | -7470A                                 |        | PPB   | 18 Sep 2020 10:46:09 | U    | SMPL |
| CCB43 - 1       | CCB43                   | -198            | -0.0332 | -7470A                                 |        | PPB   | 18 Sep 2020 10:48:25 | U    | SMPL |
| L4038-10MSD - 1 | PAV-B36-091620-10-15MSD | 13138           | 3.8403  | -7470A                                 |        | PPB   | 18 Sep 2020 10:50:42 | U    | SMPL |
| PB131699TB - 1  | PB131673TB              | -153            | -0.0202 | -7470A                                 |        | PPB   | 18 Sep 2020 10:52:59 | U    | SMPL |
| L4038-10LX5 - 1 |                         | -43             | 0.0118  | -7470A                                 |        | PPB   | 18 Sep 2020 10:55:14 | U    | SMPL |
| L4038-10A - 1   |                         | 13800           | 4.0326  | -7470A                                 |        | PPB   | 18 Sep 2020 10:57:29 | U    | SMPL |
| CCV44 - 1       | CCV44                   | 16915           | 4.9373  | -7470A                                 |        | PPB   | 18 Sep 2020 10:59:46 | U    | SMPL |
| CCB44 - 1       | CCB44                   | -189            | -0.0306 | -7470A                                 |        | PPB   | 18 Sep 2020 11:02:02 | U    | SMPL |