


LB111086

7470A

INSTRUMENT ID: CV2

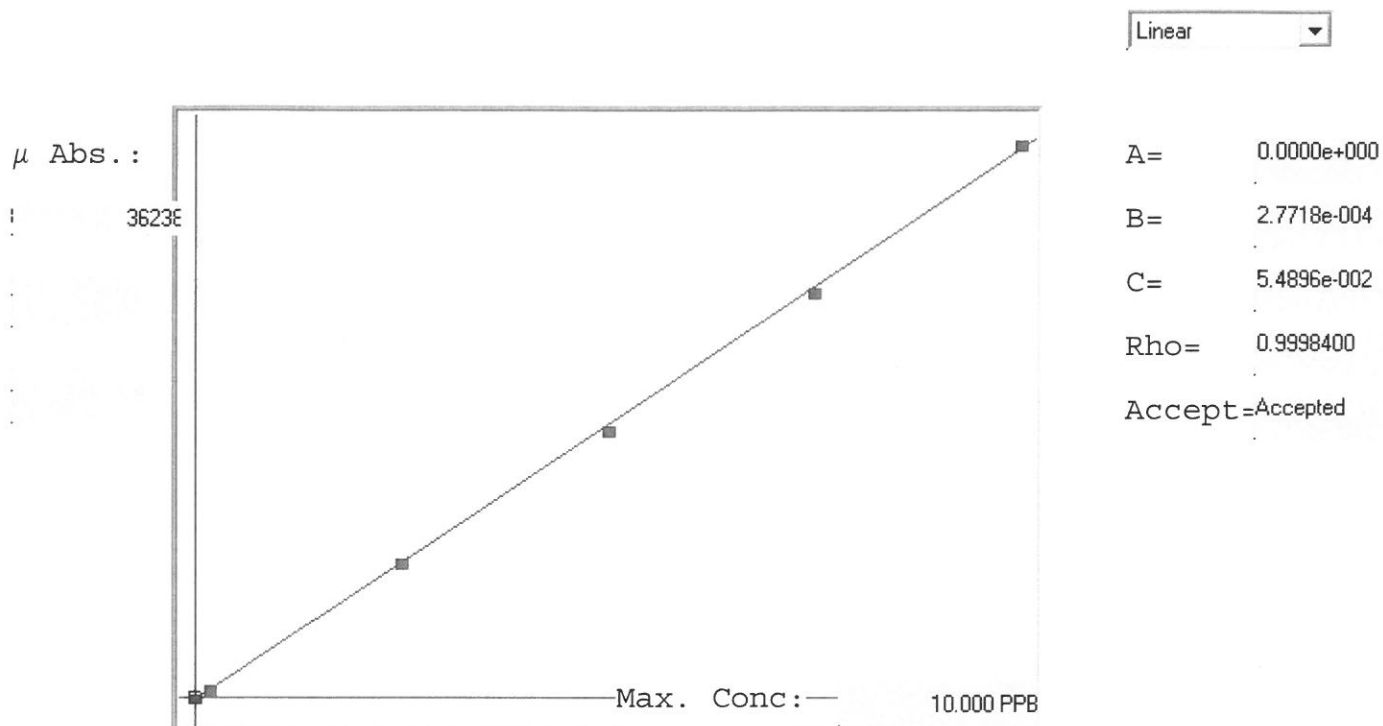

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.043	0.043	-43	0.000	-43				
0.2	0.200	0.214	0.014	574	0.0 %	574				
2.5	2.500	2.511	0.011	8862	0.0 %	8862				
5.0	5.000	4.918	-0.082	17543	0.0 %	17543				
7.5	7.500	7.415	-0.085	26552	0.0 %	26552				
10.0	10.000	10.099	0.099	36238	0.0 %	36238				

LB111086 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 22 Sep 2020 09:20:34

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-43	-	0.0000	7470A	PPB	22 Sep 2020 09:30:11	S	Std
0.2 - 1	50.2	574	-	0.2000	7470A	PPB	22 Sep 2020 09:32:27	S	Std
2.5 - 1	52.5	8862	-	2.5000	7470A	PPB	22 Sep 2020 09:34:45	S	Std
5.0 - 1	55	17543	-	5.0000	7470A	PPB	22 Sep 2020 09:37:02	S	Std
7.5 - 1	57.5	26552	-	7.5000	7470A	PPB	22 Sep 2020 09:39:18	S	Std
10.0 - 1	510	36238	-	10.0000	7470A	PPB	22 Sep 2020 09:41:34	S	Std
ICV23 - 1	ICV23	13426	3.7764	-	7470A	PPB	22 Sep 2020 09:44:18	U	SMPL
ICB23 - 1	ICB23	-194	0.0011	-	7470A	PPB	22 Sep 2020 09:46:33	U	SMPL
CCV59 - 1	CCV59	17919	5.0218	-	7470A	PPB	22 Sep 2020 09:51:32	U	SMPL
CCB59 - 1	CCB59	-187	0.0031	-	7470A	PPB	22 Sep 2020 09:53:47	U	SMPL
CRA - 1	CRA	548	0.2068	-	7470A	PPB	22 Sep 2020 09:56:02	U	SMPL
HighStd - 1	HighStd	36401	10.1447	-	7470A	PPB	22 Sep 2020 09:58:17	U	SMPL
ChkStd - 1	ChkStd	25893	7.2320	-	7470A	PPB	22 Sep 2020 10:00:33	U	SMPL
PB131757BL - 1	PBW	-277	-0.0219	-	7470A	PPB	22 Sep 2020 10:02:50	U	SMPL
PB131757BS - 1	LCSW	13249	3.7273	-	7470A	PPB	22 Sep 2020 10:05:06	U	SMPL
L3869-10 - 1	OR-02-091820	-151	0.0130	-	7470A	PPB	22 Sep 2020 10:07:22	U	SMPL
L3869-10DUP - 1	OR-02-091820DUP	-61	0.0380	-	7470A	PPB	22 Sep 2020 10:09:39	U	SMPL
L3869-10MS - 1	OR-02-091820MS	13744	3.8645	-	7470A	PPB	22 Sep 2020 10:11:56	U	SMPL
L3869-10MSD - 1	OR-02-091820MSD	13696	3.8512	-	7470A	PPB	22 Sep 2020 10:16:55	U	SMPL
L4048-02 - 1	WC-1	-168	0.0083	-	7470A	PPB	22 Sep 2020 10:19:09	U	SMPL
CCV60 - 1	CCV60	18275	5.1204	-	7470A	PPB	22 Sep 2020 10:21:25	U	SMPL
CCB60 - 1	CCB60	-187	0.0031	-	7470A	PPB	22 Sep 2020 10:23:40	U	SMPL
L4048-04 - 1	WC-2	-55	0.0397	-	7470A	PPB	22 Sep 2020 10:25:56	U	SMPL
PB131758BL - 1	PBW	-42	0.0433	-	7470A	PPB	22 Sep 2020 10:28:12	U	SMPL
PB131758BS - 1	LCSW	13763	3.8698	-	7470A	PPB	22 Sep 2020 10:30:28	U	SMPL
L4093-01 - 1	KTS-GW-01-30	121204	33.6507	-	7470A	PPB	22 Sep 2020 10:32:43	U	SMPL
L4094-01 - 1	KTS-WC-L-01	70998	19.7344	-	7470A	PPB	22 Sep 2020 10:37:59	U	SMPL
L4094-01DUP - 1	KTS-WC-L-01DUP	69570	19.3386	-	7470A	PPB	22 Sep 2020 10:40:15	U	SMPL
L4094-01MS - 1	KTS-WC-L-01MS	84885	23.5837	-	7470A	PPB	22 Sep 2020 10:49:06	U	SMPL
L4094-01MSD - 1	KTS-WC-L-01MSD	83570	23.2192	-	7470A	PPB	22 Sep 2020 10:51:22	U	SMPL
PB131757TB - 1	PB131741TB	-334	-0.0377	-	7470A	PPB	22 Sep 2020 10:53:42	U	SMPL
L4093-01DLX10 - 1		10777	3.0421	-	7470A	PPB	22 Sep 2020 10:56:00	U	SMPL
CCV61 - 1	CCV61	18188	5.0963	-	7470A	PPB	22 Sep 2020 10:58:16	U	SMPL
CCB61 - 1	CCB61	-75	0.0341	-	7470A	PPB	22 Sep 2020 11:00:32	U	SMPL
L3869-10LX5 - 1		-45	0.0424	-	7470A	PPB	22 Sep 2020 11:02:47	U	SMPL
L3869-10A - 1		14115	3.9674	-	7470A	PPB	22 Sep 2020 11:05:03	U	SMPL
L4094-01LX5 - 1		12515	3.5239	-	7470A	PPB	22 Sep 2020 11:07:18	U	SMPL
L4094-01A - 1		86334	23.9853	-	7470A	PPB	22 Sep 2020 11:09:34	U	SMPL
L4094-01DLX5 - 1		12175	3.4296	-	7470A	PPB	22 Sep 2020 11:11:51	U	SMPL
L4094-01DUPDLX5 - 1		12334	3.4737	-	7470A	PPB	22 Sep 2020 11:14:10	U	SMPL
L4094-01MSDLX5 - 1		14666	4.1201	-	7470A	PPB	22 Sep 2020 11:16:26	U	SMPL
L4094-01MSDDLX5 - 1		14810	4.1600	-	7470A	PPB	22 Sep 2020 11:18:43	U	SMPL
L4094-01LDLX25 - 1		2303	0.6933	-	7470A	PPB	22 Sep 2020 11:21:00	U	SMPL
L4094-01ADLX5 - 1		15260	4.2847	-	7470A	PPB	22 Sep 2020 11:23:16	U	SMPL
CCV62 - 1	CCV62	18448	5.1684	-	7470A	PPB	22 Sep 2020 11:25:31	U	SMPL
CCB62 - 1	CCB62	-101	0.0269	-	7470A	PPB	22 Sep 2020 11:27:47	U	SMPL