


LB111094

7471B

INSTRUMENT ID: CV1

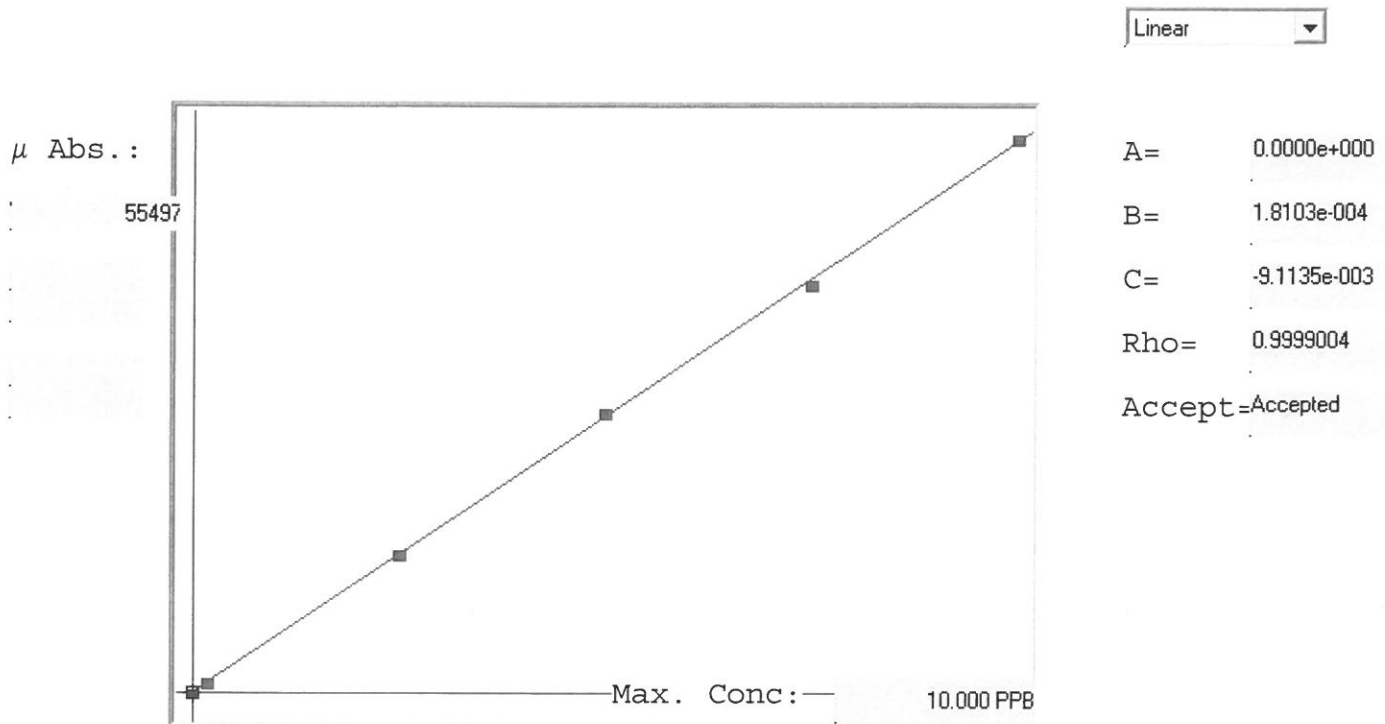

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.004	0.004	72	0.000	72				
0.2	0.200	0.188	-0.012	1091	0.0 %	1091				
2.5	2.500	2.497	-0.003	13846	0.0 %	13846				
5.0	5.000	5.071	0.071	28064	0.0 %	28064				
7.5	7.500	7.402	-0.098	40938	0.0 %	40938				
10.0	10.000	10.037	0.037	55497	0.0 %	55497				

LB111094 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 22 Sep 2020 14:46:20

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	72	-	0.0000	7471B	PPB	22 Sep 2020 14:47:56	S	Std
0.2 - 1	50.2	1091	-	0.2000	7471B	PPB	22 Sep 2020 14:50:13	S	Std
2.5 - 1	52.5	13846	-	2.5000	7471B	PPB	22 Sep 2020 14:52:30	S	Std
5.0 - 1	55	28064	-	5.0000	7471B	PPB	22 Sep 2020 14:54:47	S	Std
7.5 - 1	57.5	40938	-	7.5000	7471B	PPB	22 Sep 2020 14:57:03	S	Std
10.0 - 1	510	55497	-	10.0000	7471B	PPB	22 Sep 2020 15:04:28	S	Std
ICV24 - 1	ICV24	21552	3.8924	-	7471B	PPB	22 Sep 2020 15:07:08	U	SMPL
ICB24 - 1	ICB24	-56	-0.0193	-	7471B	PPB	22 Sep 2020 15:09:23	U	SMPL
CCV67 - 1	CCV67	28241	5.1033	-	7471B	PPB	22 Sep 2020 15:11:38	U	SMPL
CCB67 - 1	CCB67	-60	-0.0200	-	7471B	PPB	22 Sep 2020 15:13:53	U	SMPL
CRA - 1	CRA	1055	0.1819	-	7471B	PPB	22 Sep 2020 15:16:08	U	SMPL
HighStd - 1	HighStd	55290	9.9999	-	7471B	PPB	22 Sep 2020 15:18:23	U	SMPL
ChkStd - 1	ChkStd	36272	6.5571	-	7471B	PPB	22 Sep 2020 15:20:38	U	SMPL
PB131798BL - 1	PBS	-157	-0.0375	-	7471B	PPB	22 Sep 2020 15:22:55	U	SMPL
PB131798BS - 1	LCSS	18435	3.3281	-	7471B	PPB	22 Sep 2020 15:25:12	U	SMPL
L3864-08 - 1	CL-02-092120	6489	1.1656	-	7471B	PPB	22 Sep 2020 15:32:27	U	SMPL
L3864-08DUP - 1	CL-02-092120DUP	6500	1.1676	-	7471B	PPB	22 Sep 2020 15:34:44	U	SMPL
L3864-08MS - 1	CL-02-092120MS	27654	4.9970	-	7471B	PPB	22 Sep 2020 15:37:01	U	SMPL
L3864-08MSD - 1	CL-02-092120MSD	28859	5.2151	-	7471B	PPB	22 Sep 2020 15:39:18	U	SMPL
L3866-06 - 1	OK-01-092120	1319	0.2297	-	7471B	PPB	22 Sep 2020 15:41:33	U	SMPL
CCV68 - 1	CCV68	28113	5.0801	-	7471B	PPB	22 Sep 2020 15:43:48	U	SMPL
CCB68 - 1	CCB68	-18	-0.0124	-	7471B	PPB	22 Sep 2020 15:46:03	U	SMPL
L3872-07 - 1	BU-02-092120	5765	1.0345	-	7471B	PPB	22 Sep 2020 15:48:19	U	SMPL
L4099-02 - 1	029	838	0.1426	-	7471B	PPB	22 Sep 2020 15:50:34	U	SMPL
L4099-04 - 1	036	1124	0.1944	-	7471B	PPB	22 Sep 2020 15:52:50	U	SMPL
L4099-06 - 1	031	921	0.1576	-	7471B	PPB	22 Sep 2020 15:55:06	U	SMPL
L4099-08 - 1	105	1414	0.2469	-	7471B	PPB	22 Sep 2020 15:57:21	U	SMPL
L4100-02 - 1	024	4653	0.8332	-	7471B	PPB	22 Sep 2020 15:59:37	U	SMPL
L4100-04 - 1	RBR-59	713	0.1200	-	7471B	PPB	22 Sep 2020 16:01:54	U	SMPL
L4100-06 - 1	021	748	0.1263	-	7471B	PPB	22 Sep 2020 16:04:11	U	SMPL
L4101-01 - 1	0-6FT	1421	0.2481	-	7471B	PPB	22 Sep 2020 16:06:28	U	SMPL
L4104-03 - 1	PAV-B29-092120-0-10	30086	5.4373	-	7471B	PPB	22 Sep 2020 16:08:44	U	SMPL
CCV69 - 1	CCV69	28380	5.1284	-	7471B	PPB	22 Sep 2020 16:11:00	U	SMPL
CCB69 - 1	CCB69	-56	-0.0193	-	7471B	PPB	22 Sep 2020 16:13:16	U	SMPL
L4104-07 - 1	PAV-092120-DP	44755	8.0927	-	7471B	PPB	22 Sep 2020 16:15:32	U	SMPL
L4104-09 - 1	PAV-B29-092120-10-17	19262	3.4778	-	7471B	PPB	22 Sep 2020 16:17:47	U	SMPL
L3864-08LX5 - 1		1306	0.2273	-	7471B	PPB	22 Sep 2020 16:20:04	U	SMPL
L3864-08A - 1		29295	5.2941	-	7471B	PPB	22 Sep 2020 16:22:20	U	SMPL
CCV70 - 1	CCV70	28670	5.1809	-	7471B	PPB	22 Sep 2020 16:24:35	U	SMPL
CCB70 - 1	CCB70	361	0.0562	-	7471B	PPB	22 Sep 2020 16:26:52	U	SMPL