

245.1


LB111134

INSTRUMENT ID: CW1

Linear

 μ Abs.:

34468

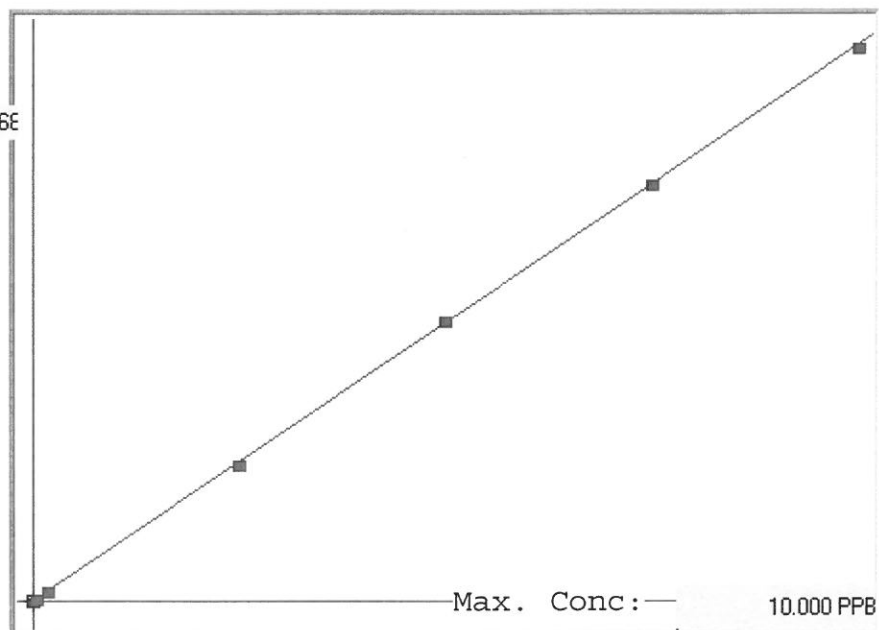

A= 0.0000e+000

B= 2.8933e-004

C= -1.2086e-003

Rho= 0.9999803

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.004	-0.004	-11	0.000	-11				
0.05	0.050	0.052	0.002	185	0.0 %	185				
0.2	0.200	0.194	-0.006	676	0.0 %	676				
2.5	2.500	2.475	-0.025	8559	0.0 %	8559				
5.0	5.000	5.045	0.045	17442	0.0 %	17442				
7.5	7.500	7.516	0.016	25981	0.0 %	25981				
10.0	10.000	9.971	-0.029	34468	0.0 %	34468				

LB111134 INSTRUMENT ID ; CV1

Method: 245.1

Operator: Admin

Date of Analysis: 24 Sep 2020 12:36:25

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	SO	-11	-	0.0000245.1	PPB	24 Sep 2020 12:38:01	S	Std
0.05 - 1	SO.07	185	-	0.0500245.1	PPB	24 Sep 2020 12:40:18	S	Std
0.2 - 1	SO.2	676	-	0.2000245.1	PPB	24 Sep 2020 12:42:36	S	Std
2.5 - 1	SO.2	8559	-	2.5000245.1	PPB	24 Sep 2020 12:44:53	S	Std
5.0 - 1	SO.2	17442	-	5.0000245.1	PPB	24 Sep 2020 12:47:09	S	Std
7.5 - 1	SO.2	25981	-	7.5000245.1	PPB	24 Sep 2020 12:49:25	S	Std
10.0 - 1	SO.2	34468	-	10.0000245.1	PPB	24 Sep 2020 12:54:17	S	Std
ICV28 - 1	ICV28	13594	3.9319	-245.1	PPB	24 Sep 2020 12:59:31	U	SMPL
ICB28 - 1	ICB28	-102	-0.0307	-245.1	PPB	24 Sep 2020 13:01:46	U	SMPL
CCV86 - 1	CCV86	17591	5.0884	-245.1	PPB	24 Sep 2020 13:04:02	U	SMPL
CCB86 - 1	CCB86	-130	-0.0388	-245.1	PPB	24 Sep 2020 13:06:17	U	SMPL
CRA - 1	CRA	147	0.0413	-245.1	PPB	24 Sep 2020 13:08:33	U	SMPL
HighStd - 1	HighStd	34965	10.1152	-245.1	PPB	24 Sep 2020 13:10:48	U	SMPL
ChkStd - 1	ChkStd	24039	6.9540	-245.1	PPB	24 Sep 2020 13:13:03	U	SMPL
PB131867BL - 1	PBW	-51	-0.0160	-245.1	PPB	24 Sep 2020 13:17:54	U	SMPL
PB131867BS - 1	LCSW	13647	3.9473	-245.1	PPB	24 Sep 2020 13:20:10	U	SMPL
L3972-08 - 1	PT-HG-WP	57716	16.6977	-245.1	PPB	24 Sep 2020 13:22:26	U	SMPL
CCV87 - 1	CCV87	16440	4.7554	-245.1	PPB	24 Sep 2020 13:33:54	U	SMPL
CCB87 - 1	CCB87	-114	-0.0342	-245.1	PPB	24 Sep 2020 13:36:11	U	SMPL
L4120-05 - 1	COMPACTOR-ELECTRICAL-SERVICE-MH	1335	0.3850	-245.1	PPB	24 Sep 2020 13:38:28	U	SMPL
L4120-08 - 1	COMPACTOR-ELECTRICAL-SERVICE-MH	-111	-0.0333	-245.1	PPB	24 Sep 2020 13:40:44	U	SMPL
CCV88 - 1	CCV88	16884	4.8838	-245.1	PPB	24 Sep 2020 13:51:49	U	SMPL
CCB88 - 1	CCB88	-82	-0.0249	-245.1	PPB	24 Sep 2020 13:56:43	U	SMPL
L4025-02 - 1	FALL-2020	1698	0.4901	-245.1	PPB	24 Sep 2020 13:58:59	U	SMPL
L4025-02DUP - 1	FALL-2020DUP	1725	0.4979	-245.1	PPB	24 Sep 2020 14:06:38	U	SMPL
L4025-02MS - 1	FALL-2020MS	13607	3.9357	-245.1	PPB	24 Sep 2020 14:08:53	U	SMPL
L4025-02MSD - 1	FALL-2020MSD	13123	3.7957	-245.1	PPB	24 Sep 2020 14:11:08	U	SMPL
L4025-02LX5 - 1		31	0.0078	-245.1	PPB	24 Sep 2020 14:13:26	U	SMPL
L4025-02A - 1		13471	3.8963	-245.1	PPB	24 Sep 2020 14:15:43	U	SMPL
L3972-08DLX5 - 1	PT-HG-WP	11008	3.1837	-245.1	PPB	24 Sep 2020 14:22:31	U	SMPL
CCV89 - 1	CCV89	16836	4.8699	-245.1	PPB	24 Sep 2020 14:27:31	U	SMPL
CCB89 - 1	CCB89	-146	-0.0435	-245.1	PPB	24 Sep 2020 14:29:48	U	SMPL