


LB111168

7471B

INSTRUMENT ID: CV1

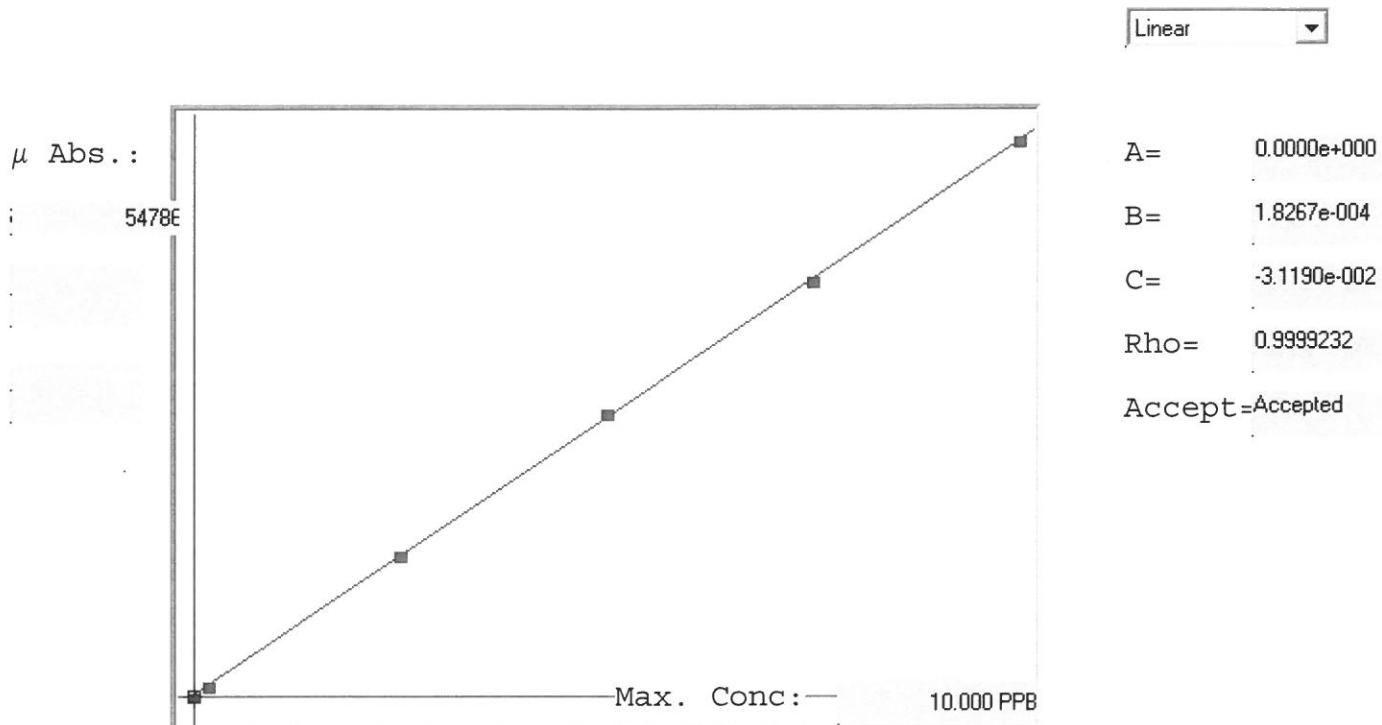

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.026	-0.026	29	0.000	29				
0.2	0.200	0.170	-0.030	1104	0.0 %	1104				
2.5	2.500	2.528	0.028	14008	0.0 %	14008				
5.0	5.000	5.090	0.090	28036	0.0 %	28036				
7.5	7.500	7.461	-0.039	41012	0.0 %	41012				
10.0	10.000	9.977	-0.023	54786	0.0 %	54786				

LB111168 INSTRUMENT ID :CV1

Method: 7471B

Operator: Admin

Date of Analysis: 25 Sep 2020 12:26:47

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	29	-	0.00007471B	PPB	25 Sep 2020 12:27:52	S	Std
0.2 - 1	50.2	1104	-	0.20007471B	PPB	25 Sep 2020 12:30:09	S	Std
2.5 - 1	52.5	14008	-	2.50007471B	PPB	25 Sep 2020 12:32:26	S	Std
5.0 - 1	55	28036	-	5.00007471B	PPB	25 Sep 2020 12:34:43	S	Std
7.5 - 1	58.5	41012	-	7.50007471B	PPB	25 Sep 2020 12:37:00	S	Std
10.0 - 1	510	54786	-	10.00007471B	PPB	25 Sep 2020 12:42:01	S	Std
ICV31 - 1	ICV31	22719	4.1190	-7471B	PPB	25 Sep 2020 12:45:52	U	SMPL
ICB31 - 1	ICB31	-98	-0.0491	-7471B	PPB	25 Sep 2020 12:48:07	U	SMPL
CCV01 - 1	CCV01	28342	5.1462	-7471B	PPB	25 Sep 2020 12:50:23	U	SMPL
CCB01 - 1	CCB01	-118	-0.0527	-7471B	PPB	25 Sep 2020 12:52:38	U	SMPL
CRA - 1	CRA	1082	0.1665	-7471B	PPB	25 Sep 2020 12:54:54	U	SMPL
HighStd - 1	HighStd	55682	10.1405	-7471B	PPB	25 Sep 2020 12:57:10	U	SMPL
ChkStd - 1	ChkStd	39360	7.1589	-7471B	PPB	25 Sep 2020 12:59:25	U	SMPL
PB131873BL - 1	PBS	-171	-0.0624	-7471B	PPB	25 Sep 2020 13:01:43	U	SMPL
PB131873BS - 1	LCSS	20110	3.6424	-7471B	PPB	25 Sep 2020 13:04:01	U	SMPL
L3871-25 - 1	TR-04-092320	9581	1.7190	-7471B	PPB	25 Sep 2020 13:06:17	U	SMPL
L3871-25DUP - 1	TR-04-092320DUP	8911	1.5966	-7471B	PPB	25 Sep 2020 13:11:08	U	SMPL
L3871-25MS - 1	TR-04-092320MS	30410	5.5239	-7471B	PPB	25 Sep 2020 13:16:09	U	SMPL
L3871-25MSD - 1	TR-04-092320MSD	29630	5.3814	-7471B	PPB	25 Sep 2020 13:18:26	U	SMPL
L4112-03 - 1	KTS-SB-0102-0-92	10395	1.8677	-7471B	PPB	25 Sep 2020 13:20:42	U	SMPL
CCV02 - 1	CCV02	27838	5.0541	-7471B	PPB	25 Sep 2020 13:22:58	U	SMPL
CCB02 - 1	CCB02	-89	-0.0474	-7471B	PPB	25 Sep 2020 13:25:13	U	SMPL
L4125-13 - 1	CS-31	972	0.1464	-7471B	PPB	25 Sep 2020 13:27:28	U	SMPL
L4125-14 - 1	CS-32	481	0.0567	-7471B	PPB	25 Sep 2020 13:29:43	U	SMPL
L4125-15 - 1	CS-33	446	0.0503	-7471B	PPB	25 Sep 2020 13:31:59	U	SMPL
L4125-16 - 1	CS-34	347	0.0322	-7471B	PPB	25 Sep 2020 13:34:14	U	SMPL
L4125-17 - 1	CS-35	356	0.0338	-7471B	PPB	25 Sep 2020 13:36:31	U	SMPL
L4125-18 - 1	CS-36	379	0.0380	-7471B	PPB	25 Sep 2020 13:38:47	U	SMPL
L4128-02 - 1	DRUM-1-5	585	0.0757	-7471B	PPB	25 Sep 2020 13:41:03	U	SMPL
L4129-16 - 1	DRUM-COMP-1	8172	1.4616	-7471B	PPB	25 Sep 2020 13:43:21	U	SMPL
L4129-17 - 1	DRUM-COMP-2	4412	0.7748	-7471B	PPB	25 Sep 2020 13:45:38	U	SMPL
L4129-18 - 1	DRUM-COMP-3	4814	0.8482	-7471B	PPB	25 Sep 2020 13:47:53	U	SMPL
CCV03 - 1	CCV03	28277	5.1343	-7471B	PPB	25 Sep 2020 13:50:09	U	SMPL
CCB03 - 1	CCB03	-62	-0.0425	-7471B	PPB	25 Sep 2020 13:52:24	U	SMPL
L4132-02 - 1	CHRT-25603	7503	1.3394	-7471B	PPB	25 Sep 2020 13:54:40	U	SMPL
L4132-04 - 1	CHRT-20413	2776	0.4759	-7471B	PPB	25 Sep 2020 13:56:55	U	SMPL
L4148-01 - 1	CTB-WEST-SOIL-(MERL)	31535	5.7294	-7471B	PPB	25 Sep 2020 13:59:11	U	SMPL
L4152-01 - 1	WR-PILE-1-2	26963	4.8943	-7471B	PPB	25 Sep 2020 14:01:27	U	SMPL
L4152-02 - 1	WR-PILE-3-4	23358	4.2357	-7471B	PPB	25 Sep 2020 14:03:44	U	SMPL
L4152-03 - 1	WR-PILE-5-7	36522	6.6404	-7471B	PPB	25 Sep 2020 14:06:00	U	SMPL
L4155-01 - 1	FK-GF-02-061-A	3714	0.6473	-7471B	PPB	25 Sep 2020 14:08:17	U	SMPL
L4155-03 - 1	FK-GF-02-061-B	5801	1.0285	-7471B	PPB	25 Sep 2020 14:10:34	U	SMPL
L3871-25LX5 - 1		1771	0.2923	-7471B	PPB	25 Sep 2020 14:12:51	U	SMPL
L3871-25A - 1		29102	5.2850	-7471B	PPB	25 Sep 2020 14:15:07	U	SMPL
CCV04 - 1	CCV04	28112	5.1041	-7471B	PPB	25 Sep 2020 14:17:22	U	SMPL
CCB04 - 1	CCB04	-50	-0.0403	-7471B	PPB	25 Sep 2020 14:19:39	U	SMPL