


LB111204

INSTRUMENT ID : CV1

7470A

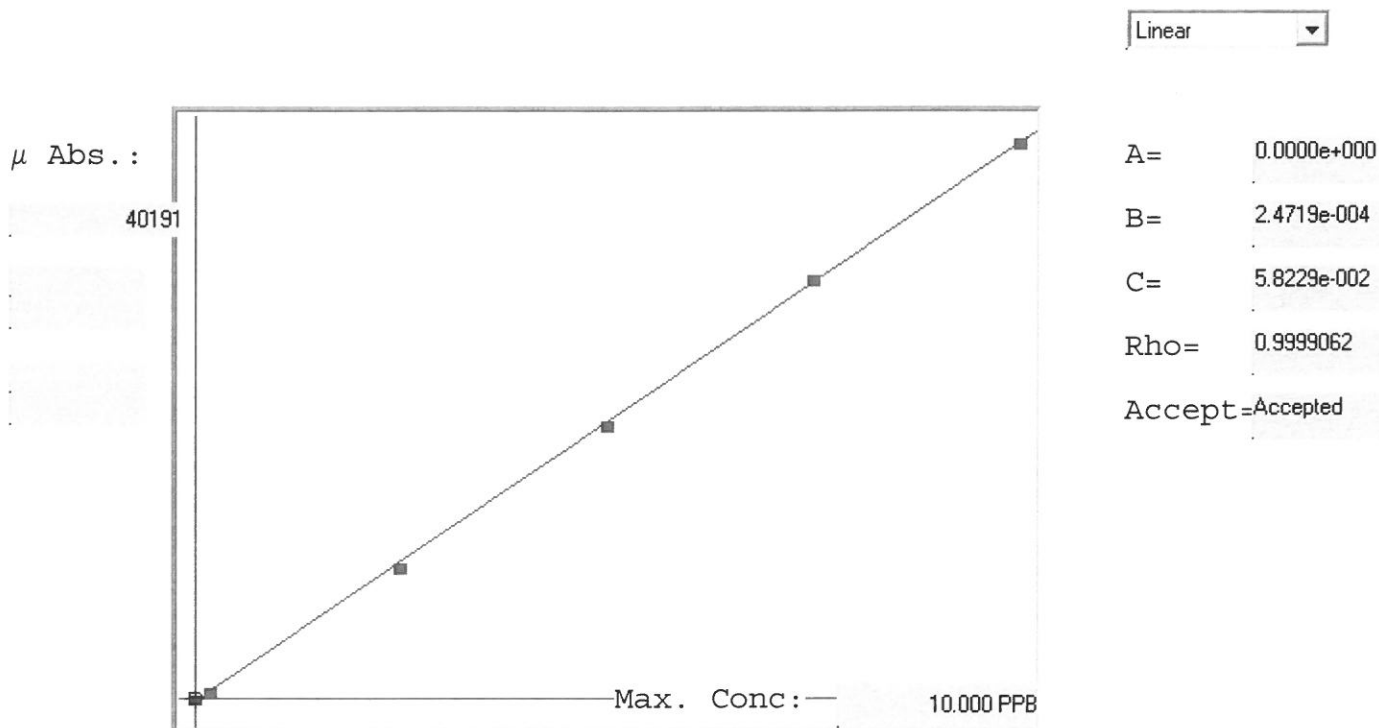

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.068	0.068	41	0.000	41				
0.2	0.200	0.195	-0.005	554	0.0 %	554				
2.5	2.500	2.421	-0.079	9559	0.0 %	9559				
5.0	5.000	4.966	-0.034	19854	0.0 %	19854				
7.5	7.500	7.556	0.056	30334	0.0 %	30334				
10.0	10.000	9.993	-0.007	40191	0.0 %	40191				

LB111204 INSTRUMENT ID : CV1

Method: 7470A	Operator: Admin	Date of Analysis: 29 Sep 2020 10:21:08							
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	41	-	0.00007470A	PPB		29 Sep 2020 10:58:00	S	Std
0.2 - 1	50.2	554	-	0.20007470A	PPB		29 Sep 2020 11:00:17	S	Std
2.5 - 1	52.5	9559	-	2.50007470A	PPB		29 Sep 2020 11:02:35	S	Std
5.0 - 1	55	19854	-	5.00007470A	PPB		29 Sep 2020 11:04:51	S	Std
7.5 - 1	57.5	30334	-	7.50007470A	PPB		29 Sep 2020 11:07:08	S	Std
10.0 - 1	510	40191	-	10.00007470A	PPB		29 Sep 2020 11:09:23	S	Std
ICV34 - 1	ICV34	14689	3.6892	-7470A	PPB		29 Sep 2020 11:12:04	U	SMPL
ICB34 - 1	ICB34	-86	0.0370	-7470A	PPB		29 Sep 2020 11:14:19	U	SMPL
CCV15 - 1	CCV15	19938	4.9867	-7470A	PPB		29 Sep 2020 11:16:34	U	SMPL
CCB15 - 1	CCB15	-92	0.0355	-7470A	PPB		29 Sep 2020 11:18:49	U	SMPL
CRA - 1	CRA	542	0.1922	-7470A	PPB		29 Sep 2020 11:21:04	U	SMPL
HighStd - 1	HighStd	39624	9.8528	-7470A	PPB		29 Sep 2020 11:23:19	U	SMPL
ChkStd - 1	ChkStd	26244	6.5455	-7470A	PPB		29 Sep 2020 11:25:35	U	SMPL
PB131953BL - 1	PBW	-213	0.0056	-7470A	PPB		29 Sep 2020 11:27:51	U	SMPL
PB131953BS - 1	LCSW	15019	3.7708	-7470A	PPB		29 Sep 2020 11:30:07	U	SMPL
L4136-04 - 1	PAV-B26-092420-0-10	-103	0.0328	-7470A	PPB		29 Sep 2020 11:32:24	U	SMPL
L4136-04DUP - 1	PAV-B26-092420-0-10DUP	-32	0.0503	-7470A	PPB		29 Sep 2020 11:34:40	U	SMPL
L4136-04MS - 1	PAV-B26-092420-0-10MS	14487	3.6393	-7470A	PPB		29 Sep 2020 11:36:57	U	SMPL
L4136-04MSD - 1	PAV-B26-092420-0-10MSD	14540	3.6524	-7470A	PPB		29 Sep 2020 11:39:14	U	SMPL
L4136-06 - 1	PAV-B26-092420-10-19	-98	0.0340	-7470A	PPB		29 Sep 2020 11:41:29	U	SMPL
CCV16 - 1	CCV16	20079	5.0215	-7470A	PPB		29 Sep 2020 11:43:45	U	SMPL
CCB16 - 1	CCB16	-67	0.0417	-7470A	PPB		29 Sep 2020 11:46:00	U	SMPL
PB131954BL - 1	PBW	-8	0.0563	-7470A	PPB		29 Sep 2020 11:48:15	U	SMPL
PB131954BS - 1	LCSW	14650	3.6795	-7470A	PPB		29 Sep 2020 11:50:30	U	SMPL
L4158-05 - 1	BLUE-FRAC-TANK	-53	0.0451	-7470A	PPB		29 Sep 2020 11:52:46	U	SMPL
L4158-05DUP - 1	BLUE-FRAC-TANKDUP	-16	0.0543	-7470A	PPB		29 Sep 2020 11:55:01	U	SMPL
L4158-05MS - 1	BLUE-FRAC-TANKMS	15241	3.8256	-7470A	PPB		29 Sep 2020 11:57:17	U	SMPL
L4158-05MSD - 1	BLUE-FRAC-TANKMSD	14675	3.6857	-7470A	PPB		29 Sep 2020 11:59:33	U	SMPL
PB131955BL - 1	PBW	-131	0.0258	-7470A	PPB		29 Sep 2020 12:01:50	U	SMPL
PB131955BS - 1	LCSW	14309	3.5953	-7470A	PPB		29 Sep 2020 12:04:07	U	SMPL
L4158-04 - 1	BLUE-FRAC-TANK	267	0.1242	-7470A	PPB		29 Sep 2020 12:11:15	U	SMPL
L4158-04DUP - 1	BLUE-FRAC-TANKDUP	213	0.1109	-7470A	PPB		29 Sep 2020 12:13:31	U	SMPL
CCV17 - 1	CCV17	19560	4.8932	-7470A	PPB		29 Sep 2020 12:15:46	U	SMPL
CCB17 - 1	CCB17	-21	0.0530	-7470A	PPB		29 Sep 2020 12:18:02	U	SMPL
L4158-04MS - 1	BLUE-FRAC-TANKMS	15165	3.8068	-7470A	PPB		29 Sep 2020 12:20:17	U	SMPL
L4158-04MSD - 1	BLUE-FRAC-TANKMSD	15732	3.9470	-7470A	PPB		29 Sep 2020 12:22:32	U	SMPL
PB131953TB - 1	PB131913TB	-102	0.0330	-7470A	PPB		29 Sep 2020 12:24:49	U	SMPL
PB131954TB - 1	PB131920TB	33	0.0664	-7470A	PPB		29 Sep 2020 12:27:04	U	SMPL
L4136-04LX5 - 1		-15	0.0545	-7470A	PPB		29 Sep 2020 13:49:21	U	SMPL
L4136-04A - 1		15450	3.8773	-7470A	PPB		29 Sep 2020 13:51:36	U	SMPL
L4158-05LX5 - 1		-81	0.0382	-7470A	PPB		29 Sep 2020 13:53:53	U	SMPL
L4158-05A - 1		15962	4.0039	-7470A	PPB		29 Sep 2020 13:56:10	U	SMPL
L4158-04LX5 - 1		-7	0.0565	-7470A	PPB		29 Sep 2020 13:58:26	U	SMPL
L4158-04A - 1		15915	3.9922	-7470A	PPB		29 Sep 2020 14:00:42	U	SMPL
CCV18 - 1	CCV18	19497	4.8777	-7470A	PPB		29 Sep 2020 14:02:58	U	SMPL
CCB18 - 1	CCB18	-124	0.0276	-7470A	PPB		29 Sep 2020 14:05:14	U	SMPL