


LB111220

7470A

INSTRUMENT ID: CV1

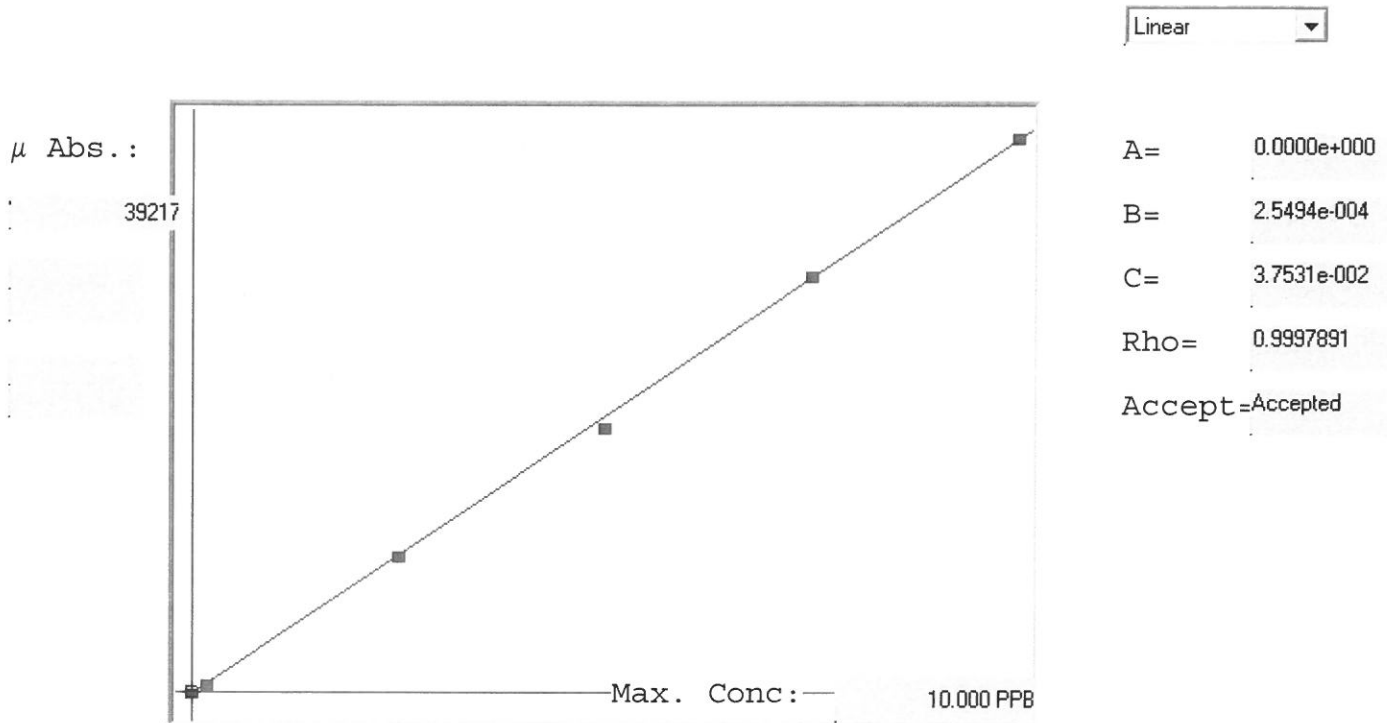

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.060	0.060	89	0.000	89				
0.2	0.200	0.210	0.010	677	0.0 %	677				
2.5	2.500	2.501	0.001	9662	0.0 %	9662				
5.0	5.000	4.838	-0.162	18828	0.0 %	18828				
7.5	7.500	7.556	0.056	29489	0.0 %	29489				
10.0	10.000	10.036	0.036	39217	0.0 %	39217				

LB111220 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 30 Sep 2020 09:21:22

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	90	89	-	0.0000	7470A	PPB	30 Sep 2020 09:21:30	S	Std
0.2 - 1	50.2	677	-	0.2000	7470A	PPB	30 Sep 2020 09:23:48	S	Std
2.5 - 1	52.5	9662	-	2.5000	7470A	PPB	30 Sep 2020 09:26:05	S	Std
5.0 - 1	55	18828	-	5.0000	7470A	PPB	30 Sep 2020 09:28:22	S	Std
7.5 - 1	57.5	29489	-	7.5000	7470A	PPB	30 Sep 2020 09:30:38	S	Std
10.0 - 1	510	39217	-	10.0000	7470A	PPB	30 Sep 2020 09:32:54	S	Std
ICV36 - 1	ICV36	14594	3.7582	-	7470A	PPB	30 Sep 2020 09:38:24	U	SMPL
ICB36 - 1	ICB36	-8	0.0355	-	7470A	PPB	30 Sep 2020 09:40:39	U	SMPL
CCV22 - 1	CCV22	19107	4.9087	-	7470A	PPB	30 Sep 2020 09:42:54	U	SMPL
CCB22 - 1	CCB22	-31	0.0296	-	7470A	PPB	30 Sep 2020 09:45:09	U	SMPL
CRA - 1	CRA	653	0.2040	-	7470A	PPB	30 Sep 2020 09:47:24	U	SMPL
HighStd - 1	HighStd	39512	10.1109	-	7470A	PPB	30 Sep 2020 09:49:40	U	SMPL
ChkStd - 1	ChkStd	23724	6.0858	-	7470A	PPB	30 Sep 2020 09:51:55	U	SMPL
PB131981BL - 1	PBW	-77	0.0179	-	7470A	PPB	30 Sep 2020 09:54:12	U	SMPL
PB131981BS - 1	LCSW	15017	3.8660	-	7470A	PPB	30 Sep 2020 09:56:28	U	SMPL
L3867-12 - 1	EO-01-092820	-10	0.0350	-	7470A	PPB	30 Sep 2020 09:58:44	U	SMPL
L3867-12DUP - 1	EO-01-092820DUP	86	0.0595	-	7470A	PPB	30 Sep 2020 10:01:01	U	SMPL
L3867-12MS - 1	EO-01-092820MS	14793	3.8089	-	7470A	PPB	30 Sep 2020 10:03:18	U	SMPL
L3867-12MSD - 1	EO-01-092820MSD	14875	3.8298	-	7470A	PPB	30 Sep 2020 10:05:35	U	SMPL
L3869-15 - 1	OR-03-092820	-58	0.0227	-	7470A	PPB	30 Sep 2020 10:07:50	U	SMPL
CCV23 - 1	CCV23	19155	4.9210	-	7470A	PPB	30 Sep 2020 10:10:05	U	SMPL
CCB23 - 1	CCB23	-19	0.0327	-	7470A	PPB	30 Sep 2020 10:12:20	U	SMPL
L4173-03 - 1	TP-1-(0-6FT)	36	0.0467	-	7470A	PPB	30 Sep 2020 10:14:36	U	SMPL
L4173-07 - 1	TP-2-(0-6FT)	12	0.0406	-	7470A	PPB	30 Sep 2020 10:16:52	U	SMPL
L4173-11 - 1	TP-3-(0-6FT)	60	0.0528	-	7470A	PPB	30 Sep 2020 10:19:07	U	SMPL
PB131982BL - 1	PBW	127	0.0699	-	7470A	PPB	30 Sep 2020 10:21:23	U	SMPL
PB131982BS - 1	LCSW	15709	4.0424	-	7470A	PPB	30 Sep 2020 10:23:38	U	SMPL
L4189-03 - 1	TP-C-2334-GW	3318	0.8834	-	7470A	PPB	30 Sep 2020 10:25:54	U	SMPL
L4189-03DUP - 1	TP-C-2334-GWDUP	3032	0.8105	-	7470A	PPB	30 Sep 2020 10:28:11	U	SMPL
L4189-03MS - 1	TP-C-2334-GWMS	18786	4.8269	-	7470A	PPB	30 Sep 2020 10:30:28	U	SMPL
L4189-03MSD - 1	TP-C-2334-GWMSD	18685	4.8012	-	7470A	PPB	30 Sep 2020 10:32:45	U	SMPL
CCV24 - 1	CCV24	18808	4.8325	-	7470A	PPB	30 Sep 2020 10:35:01	U	SMPL
CCB24 - 1	CCB24	-10	0.0350	-	7470A	PPB	30 Sep 2020 10:37:17	U	SMPL
PB131981TB - 1	PB131945TB	99	0.0628	-	7470A	PPB	30 Sep 2020 10:39:32	U	SMPL
L4189-03LX5 - 1		71	0.0556	-	7470A	PPB	30 Sep 2020 10:41:48	U	SMPL
L4189-03A - 1		14542	3.7449	-	7470A	PPB	30 Sep 2020 10:44:04	U	SMPL
L3867-12LX5 - 1		569	0.1826	-	7470A	PPB	30 Sep 2020 10:46:19	U	SMPL
L3867-12A - 1		18427	4.7354	-	7470A	PPB	30 Sep 2020 10:48:35	U	SMPL
CCV25 - 1	CCV25	18766	4.8218	-	7470A	PPB	30 Sep 2020 10:50:51	U	SMPL
CCB25 - 1	CCB25	-2	0.0370	-	7470A	PPB	30 Sep 2020 10:53:08	U	SMPL