


LB111267

7471B

INSTRUMENT ID: CV1

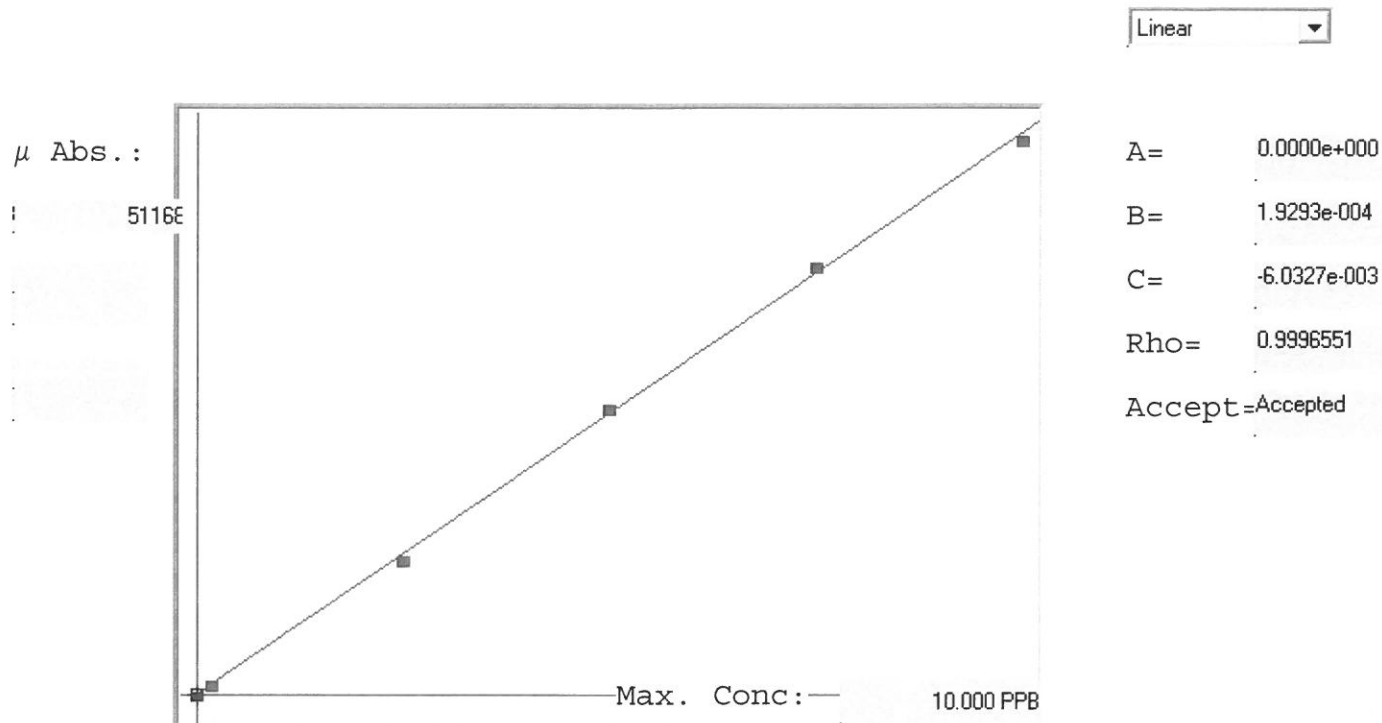

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.023	0.023	148	0.000	148				
0.2	0.200	0.166	-0.034	893	0.0 %	893				
2.5	2.500	2.410	-0.090	12522	0.0 %	12522				
5.0	5.000	5.100	0.100	26464	0.0 %	26464				
7.5	7.500	7.636	0.136	39613	0.0 %	39613				
10.0	10.000	9.866	-0.134	51168	0.0 %	51168				

LB111267 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 02 Oct 2020 11:13:31

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	148	-	0.0000	7471B	PPB	02 Oct 2020 11:15:22	S	Std
0.2 - 1	50.2	893	-	0.2000	7471B	PPB	02 Oct 2020 11:17:39	S	Std
2.5 - 1	52.5	12522	-	2.5000	7471B	PPB	02 Oct 2020 11:19:56	S	Std
5.0 - 1	55	26464	-	5.0000	7471B	PPB	02 Oct 2020 11:22:13	S	Std
7.5 - 1	57.5	39613	-	7.5000	7471B	PPB	02 Oct 2020 11:24:30	S	Std
10.0 - 1	518	51168	-	10.0000	7471B	PPB	02 Oct 2020 11:26:46	S	Std
ICV40 - 1	ICV40	19369	3.7307	-	7471B	PPB	02 Oct 2020 11:29:32	U	SMPL
ICB40 - 1	ICB40	-104	-0.0261	-	7471B	PPB	02 Oct 2020 11:31:47	U	SMPL
CCV42 - 1	CCV42	27565	5.3120	-	7471B	PPB	02 Oct 2020 11:34:01	U	SMPL
CCB42 - 1	CCB42	-109	-0.0271	-	7471B	PPB	02 Oct 2020 11:36:17	U	SMPL
CRA - 1	CRA	894	0.1664	-	7471B	PPB	02 Oct 2020 11:38:33	U	SMPL
HighStd - 1	HighStd	51365	9.9036	-	7471B	PPB	02 Oct 2020 11:40:48	U	SMPL
ChkStd - 1	ChkStd	36650	7.0647	-	7471B	PPB	02 Oct 2020 11:43:03	U	SMPL
PB132036BL - 1	PBS	-148	-0.0346	-	7471B	PPB	02 Oct 2020 11:45:22	U	SMPL
PB132036BS - 1	LCSS	17694	3.4076	-	7471B	PPB	02 Oct 2020 11:47:39	U	SMPL
L3865-01 - 1	NB-08-093020	6359	1.2208	-	7471B	PPB	02 Oct 2020 11:49:55	U	SMPL
L3865-05 - 1	NB-07-093020	4355	0.8342	-	7471B	PPB	02 Oct 2020 11:52:12	U	SMPL
L3872-13 - 1	BU-03-093020	2454	0.4674	-	7471B	PPB	02 Oct 2020 11:54:30	U	SMPL
L4194-01 - 1	CG-SOIL	1372	0.2587	-	7471B	PPB	02 Oct 2020 11:56:47	U	SMPL
L4195-02 - 1	RBR-200010	298	0.0515	-	7471B	PPB	02 Oct 2020 11:59:02	U	SMPL
CCV43 - 1	CCV43	26809	5.1661	-	7471B	PPB	02 Oct 2020 12:01:17	U	SMPL
CCB43 - 1	CCB43	-94	-0.0242	-	7471B	PPB	02 Oct 2020 12:03:33	U	SMPL
L4195-04 - 1	RBR-251673	1820	0.3451	-	7471B	PPB	02 Oct 2020 12:05:48	U	SMPL
L4196-02 - 1	RBR-251609	650	0.1194	-	7471B	PPB	02 Oct 2020 12:08:03	U	SMPL
L4198-01 - 1	RO-15	1985	0.3769	-	7471B	PPB	02 Oct 2020 12:10:19	U	SMPL
L4198-04 - 1	RO-21	2171	0.4128	-	7471B	PPB	02 Oct 2020 12:12:34	U	SMPL
L4198-07 - 1	RO-25	4659	0.8928	-	7471B	PPB	02 Oct 2020 12:14:52	U	SMPL
L4198-10 - 1	RO-24	5354	1.0269	-	7471B	PPB	02 Oct 2020 12:17:08	U	SMPL
L4198-13 - 1	RO-10	4765	0.9133	-	7471B	PPB	02 Oct 2020 12:19:24	U	SMPL
L4198-16 - 1	RO-5	3411	0.6520	-	7471B	PPB	02 Oct 2020 12:21:41	U	SMPL
L4198-19 - 1	RO-20	9299	1.7880	-	7471B	PPB	02 Oct 2020 12:23:58	U	SMPL
L4198-22 - 1	RO-17	8359	1.6066	-	7471B	PPB	02 Oct 2020 12:26:13	U	SMPL
CCV44 - 1	CCV44	27526	5.3044	-	7471B	PPB	02 Oct 2020 12:28:29	U	SMPL
CCB44 - 1	CCB44	-94	-0.0242	-	7471B	PPB	02 Oct 2020 12:30:44	U	SMPL
L4198-28 - 1	RO-19	1158	0.2174	-	7471B	PPB	02 Oct 2020 12:33:00	U	SMPL
L4198-31 - 1	RO-4	5115	0.9808	-	7471B	PPB	02 Oct 2020 12:35:15	U	SMPL
L4199-01 - 1	11940	4323	0.8280	-	7471B	PPB	02 Oct 2020 12:37:31	U	SMPL
L4199-01DUP - 1	11940DUP	4173	0.7990	-	7471B	PPB	02 Oct 2020 12:39:46	U	SMPL
L4199-01MS - 1	11940MS	24665	4.7525	-	7471B	PPB	02 Oct 2020 12:42:02	U	SMPL
L4199-01MSD - 1	11940MSD	23837	4.5927	-	7471B	PPB	02 Oct 2020 12:44:19	U	SMPL
L4199-01LX5 - 1		762	0.1410	-	7471B	PPB	02 Oct 2020 12:46:35	U	SMPL
L4199-01A - 1		24925	4.8026	-	7471B	PPB	02 Oct 2020 12:48:52	U	SMPL
CCV45 - 1	CCV45	27224	5.2462	-	7471B	PPB	02 Oct 2020 12:51:09	U	SMPL
CCB45 - 1	CCB45	-98	-0.0249	-	7471B	PPB	02 Oct 2020 12:53:26	U	SMPL