


LB 111326

7470A

INSTRUMENT ID: CV1

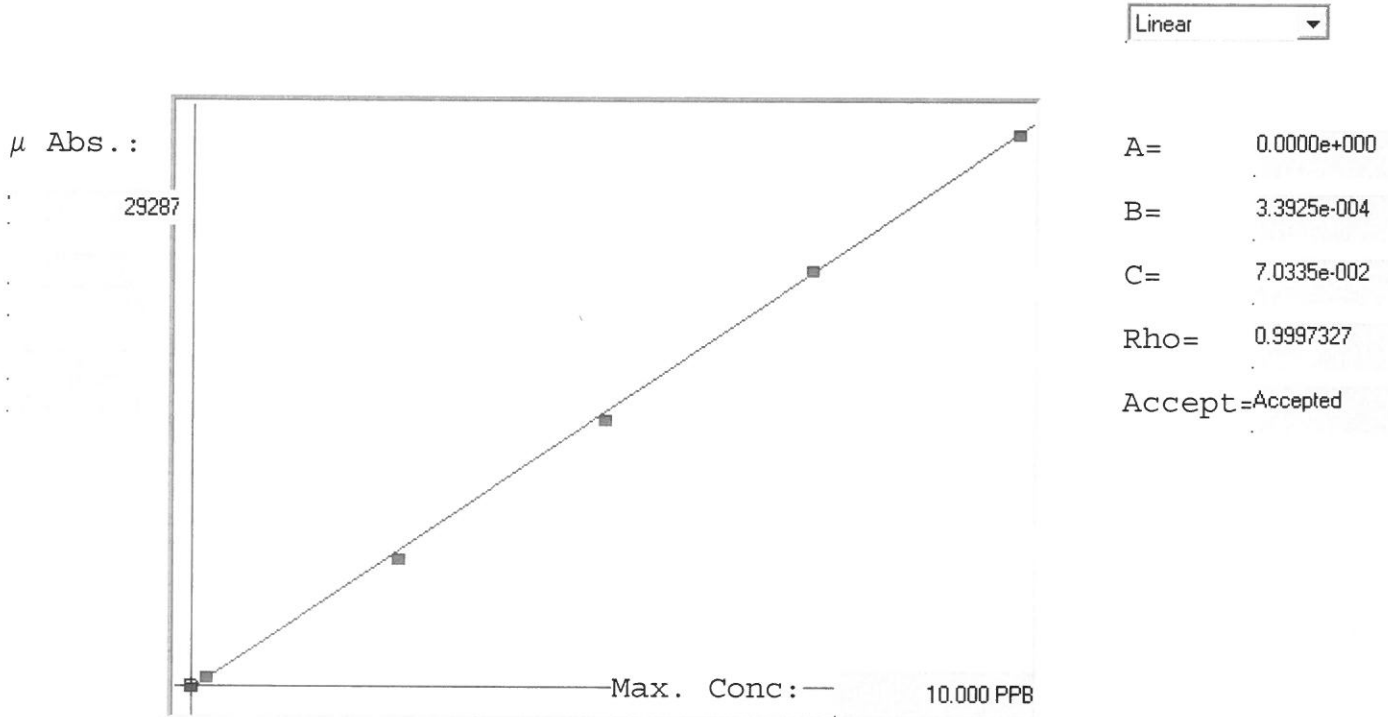

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.074	0.074	11	0.000	11				
0.2	0.200	0.249	0.049	526	0.0 %	526				
2.5	2.500	2.387	-0.113	6828	0.0 %	6828				
5.0	5.000	4.885	-0.115	14193	0.0 %	14193				
7.5	7.500	7.599	0.099	22192	0.0 %	22192				
10.0	10.000	10.006	0.006	29287	0.0 %	29287				

LB111326 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 06 Oct 2020 10:08:23

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	11	-	0.0000	7470A	PPB	06 Oct 2020 10:40:57	S	Std
0.2 - 1	50.2	526	-	0.2000	7470A	PPB	06 Oct 2020 10:43:14	S	Std
2.5 - 1	52.5	6828	-	2.5000	7470A	PPB	06 Oct 2020 10:45:31	S	Std
5.0 - 1	55	14193	-	5.0000	7470A	PPB	06 Oct 2020 10:47:48	S	Std
7.5 - 1	57.5	22192	-	7.5000	7470A	PPB	06 Oct 2020 10:50:04	S	Std
10.0 - 1	510	29287	-	10.0000	7470A	PPB	06 Oct 2020 10:52:20	S	Std
ICV43 - 1	ICV43	10866	3.7567	-	7470A	PPB	06 Oct 2020 10:55:38	U	SMPL
ICB43 - 1	ICB43	-124	0.0283	-	7470A	PPB	06 Oct 2020 10:57:52	U	SMPL
CCV59 - 1	CCV59	13879	4.7788	-	7470A	PPB	06 Oct 2020 11:00:07	U	SMPL
CCB59 - 1	CCB59	-119	0.0300	-	7470A	PPB	06 Oct 2020 11:02:22	U	SMPL
CRA - 1	CRA	505	0.2417	-	7470A	PPB	06 Oct 2020 11:04:37	U	SMPL
HighStd - 1	HighStd	28116	9.6088	-	7470A	PPB	06 Oct 2020 11:06:52	U	SMPL
ChkStd - 1	ChkStd	20031	6.8659	-	7470A	PPB	06 Oct 2020 11:09:07	U	SMPL
PB132112BL - 1	PBW	-184	0.0079	-	7470A	PPB	06 Oct 2020 11:11:24	U	SMPL
PB132112BS - 1	LCSW	10402	3.5992	-	7470A	PPB	06 Oct 2020 11:13:41	U	SMPL
L4260-04 - 1	PAV-B21-100220-0-10	-105	0.0347	-	7470A	PPB	06 Oct 2020 11:15:57	U	SMPL
L4260-04DUP - 1	PAV-B21-100220-0-10DUP	-28	0.0608	-	7470A	PPB	06 Oct 2020 11:18:14	U	SMPL
L4260-04MS - 1	PAV-B21-100220-0-10MS	12911	4.4504	-	7470A	PPB	06 Oct 2020 11:20:31	U	SMPL
L4260-04MSD - 1	PAV-B21-100220-0-10MSD	11750	4.0566	-	7470A	PPB	06 Oct 2020 11:22:47	U	SMPL
L4260-06 - 1	PAV-B21-100220-10-18.5	-115	0.0313	-	7470A	PPB	06 Oct 2020 11:25:04	U	SMPL
CCV60 - 1	CCV60	14677	5.0495	-	7470A	PPB	06 Oct 2020 11:27:19	U	SMPL
CCB60 - 1	CCB60	-119	0.0300	-	7470A	PPB	06 Oct 2020 11:29:34	U	SMPL
L4260-12 - 1	PAV-B23-100220-0-10	-28	0.0608	-	7470A	PPB	06 Oct 2020 11:31:50	U	SMPL
L4260-14 - 1	PAV-B23-100220-10-19	-3	0.0693	-	7470A	PPB	06 Oct 2020 11:34:06	U	SMPL
L4264-01 - 1	BPC-WASTE-DRUM	-7	0.0680	-	7470A	PPB	06 Oct 2020 11:36:22	U	SMPL
PB132113BL - 1	PBW	-31	0.0598	-	7470A	PPB	06 Oct 2020 11:38:38	U	SMPL
PB132113BS - 1	LCSW	12627	4.3541	-	7470A	PPB	06 Oct 2020 11:40:53	U	SMPL
L4260-17 - 1	FIELD-BLANK	-138	0.0235	-	7470A	PPB	06 Oct 2020 11:43:09	U	SMPL
PB132112TB - 1	PB132088TB	-14	0.0656	-	7470A	PPB	06 Oct 2020 11:45:26	U	SMPL
L4260-04LX5 - 1		-14	0.0656	-	7470A	PPB	06 Oct 2020 11:47:43	U	SMPL
L4260-04A - 1		11575	3.9972	-	7470A	PPB	06 Oct 2020 11:50:00	U	SMPL
CCV61 - 1	CCV61	13238	4.5614	-	7470A	PPB	06 Oct 2020 11:52:16	U	SMPL
CCB61 - 1	CCB61	-119	0.0300	-	7470A	PPB	06 Oct 2020 11:54:32	U	SMPL