


LB111331

7470A

INSTRUMENT ID: CV1

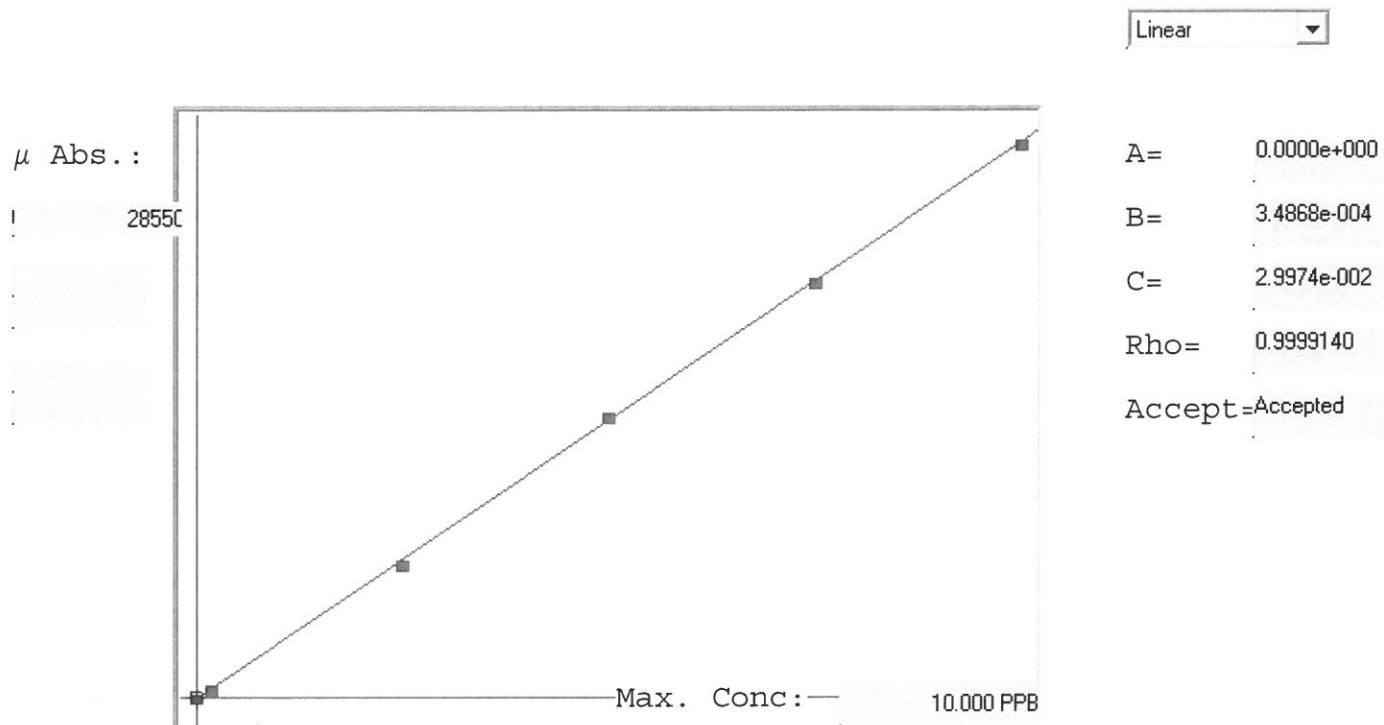

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.025	0.025	-13	0.000	-13				
0.2	0.200	0.195	-0.005	473	0.0 %	473				
2.5	2.500	2.423	-0.077	6862	0.0 %	6862				
5.0	5.000	5.084	0.084	14494	0.0 %	14494				
7.5	7.500	7.488	-0.012	21390	0.0 %	21390				
10.0	10.000	9.985	-0.015	28550	0.0 %	28550				

LB111331 INSTRUMENT ID ; CV1

Method: 7470A		Operator: Admin		Date of Analysis: 06 Oct 2020 14:54:53				
Sample ID	Extended ID	μ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	-13	-	0.00007470A	PPB	06 Oct 2020 14:56:24	S	Std
0.2 - 1	50.2	473	-	0.20007470A	PPB	06 Oct 2020 14:58:41	S	Std
2.5 - 1	52.5	6862	-	2.50007470A	PPB	06 Oct 2020 15:00:58	S	Std
5.0 - 1	55	14494	-	5.00007470A	PPB	06 Oct 2020 15:03:14	S	Std
7.5 - 1	57.5	21390	-	7.50007470A	PPB	06 Oct 2020 15:05:31	S	Std
10.0 - 1	57.5	28550	-	10.00007470A	PPB	06 Oct 2020 15:10:23	S	Std
ICV44 - 1	ICV44	11648	4.0914	-7470A	PPB	06 Oct 2020 15:15:29	U	SMPL
ICB44 - 1	ICB44	-200	-0.0398	-7470A	PPB	06 Oct 2020 15:17:44	U	SMPL
CCV62 - 1	CCV62	13676	4.7986	-7470A	PPB	06 Oct 2020 15:20:00	U	SMPL
CCB62 - 1	CCB62	-117	-0.0108	-7470A	PPB	06 Oct 2020 15:22:15	U	SMPL
CRA - 1	CRA	428	0.1792	-7470A	PPB	06 Oct 2020 15:24:31	U	SMPL
HighStd - 1	HighStd	26634	9.3168	-7470A	PPB	06 Oct 2020 15:26:46	U	SMPL
ChkStd - 1	ChkStd	19364	6.7819	-7470A	PPB	06 Oct 2020 15:29:01	U	SMPL
PB132154BL - 1	PBW	-155	-0.0241	-7470A	PPB	06 Oct 2020 15:31:19	U	SMPL
PB132154BS - 1	LCSW	9875	3.4732	-7470A	PPB	06 Oct 2020 15:33:36	U	SMPL
L4219-08 - 1	CL-01-100120	-109	-0.0080	-7470A	PPB	06 Oct 2020 15:35:53	U	SMPL
L4219-08DUP - 1	CL-01-100120DUP	-33	0.0185	-7470A	PPB	06 Oct 2020 15:38:09	U	SMPL
L4219-08MS - 1	CL-01-100120MS	9583	3.3714	-7470A	PPB	06 Oct 2020 15:40:26	U	SMPL
L4219-08MSD - 1	CL-01-100120MSD	9608	3.3801	-7470A	PPB	06 Oct 2020 15:42:43	U	SMPL
L4221-05 - 1	OK-02-100120	-26	0.0209	-7470A	PPB	06 Oct 2020 15:46:31	U	SMPL
CCV63 - 1	CCV63	15492	5.4318	-7470A	PPB	06 Oct 2020 15:59:21	U	SMPL
CCB63 - 1	CCB63	-113	-0.0094	-7470A	PPB	06 Oct 2020 16:01:37	U	SMPL
L4226-04 - 1	TR-05-100120	-41	0.0157	-7470A	PPB	06 Oct 2020 16:03:52	U	SMPL
PB132154TB - 1	PB132062TB	-31	0.0192	-7470A	PPB	06 Oct 2020 16:06:07	U	SMPL
L4219-08LX5 - 1		-43	0.0150	-7470A	PPB	06 Oct 2020 16:08:23	U	SMPL
L4219-08A - 1		12470	4.3781	-7470A	PPB	06 Oct 2020 16:15:29	U	SMPL
CCV64 - 1	CCV64	14933	5.2369	-7470A	PPB	06 Oct 2020 16:17:45	U	SMPL
CCB64 - 1	CCB64	-122	-0.0126	-7470A	PPB	06 Oct 2020 16:20:01	U	SMPL