


LB111335

7471B

INSTRUMENT ID: CV1

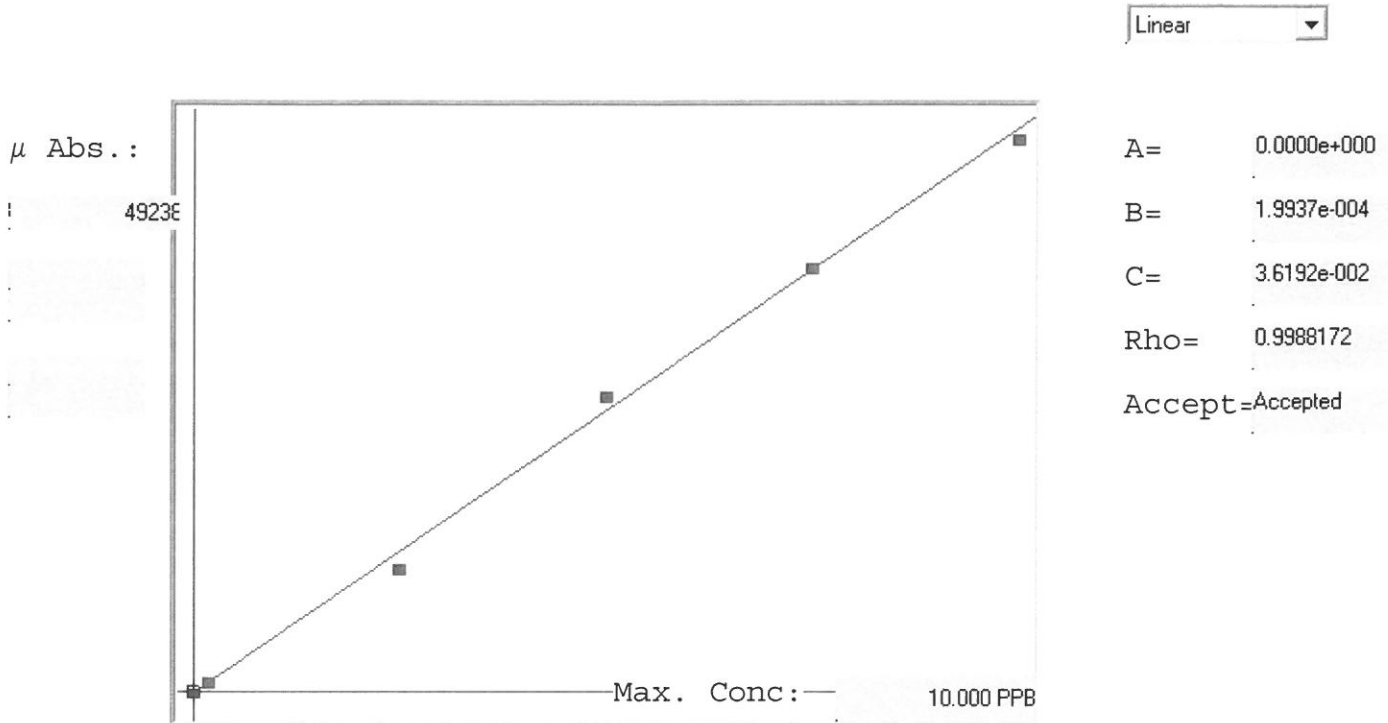

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.035	0.035	-6	0.000	-6				
0.2	0.200	0.233	0.033	987	0.0 %	987				
2.5	2.500	2.218	-0.282	10946	0.0 %	10946				
5.0	5.000	5.292	0.292	26361	0.0 %	26361				
7.5	7.500	7.569	0.069	37784	0.0 %	37784				
10.0	10.000	9.853	-0.147	49238	0.0 %	49238				

LB111335 INSTRUMENT ID : CV1

Method: 7471B	Operator: Admin	Date of Analysis: 06 Oct 2020 16:36:58							
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-6	-	0.0000	7471B	PPB	06 Oct 2020 16:37:16	S	Std
0.2 - 1	50.2	987	-	0.2000	7471B	PPB	06 Oct 2020 16:39:33	S	Std
2.5 - 1	52.5	10946	-	2.5000	7471B	PPB	06 Oct 2020 16:41:50	S	Std
5.0 - 1	55	26361	-	5.0000	7471B	PPB	06 Oct 2020 16:44:07	S	Std
7.5 - 1	57.5	37784	-	7.5000	7471B	PPB	06 Oct 2020 16:46:24	S	Std
10.0 - 1	510	49238	-	10.0000	7471B	PPB	06 Oct 2020 16:51:15	S	Std
ICV45 - 1	ICV45	18482	3.7209	-	7471B	PPB	06 Oct 2020 16:54:22	U	SMPL
ICB45 - 1	ICB45	-79	0.0204	-	7471B	PPB	06 Oct 2020 17:01:52	U	SMPL
CCV65 - 1	CCV65	24411	4.9030	-	7471B	PPB	06 Oct 2020 17:06:37	U	SMPL
CCB65 - 1	CCB65	-163	0.0037	-	7471B	PPB	06 Oct 2020 17:08:52	U	SMPL
CRA - 1	CRA	815	0.1987	-	7471B	PPB	06 Oct 2020 17:11:08	U	SMPL
HighStd - 1	HighStd	49369	9.8788	-	7471B	PPB	06 Oct 2020 17:13:23	U	SMPL
ChkStd - 1	ChkStd	36521	7.3173	-	7471B	PPB	06 Oct 2020 17:15:39	U	SMPL
PB132137BL - 1	PBS	-147	0.0069	-	7471B	PPB	06 Oct 2020 17:17:56	U	SMPL
PB132137BS - 1	LCSS	18394	3.7034	-	7471B	PPB	06 Oct 2020 17:20:13	U	SMPL
L4272-01 - 1	MH-1-(6)	2448	0.5242	-	7471B	PPB	06 Oct 2020 17:22:30	U	SMPL
L4272-01DUP - 1	MH-1-(6)DUP	2277	0.4902	-	7471B	PPB	06 Oct 2020 17:24:46	U	SMPL
L4272-01MS - 1	MH-1-(6)MS	20977	4.2183	-	7471B	PPB	06 Oct 2020 17:27:03	U	SMPL
L4272-01MSD - 1	MH-1-(6)MSD	20542	4.1316	-	7471B	PPB	06 Oct 2020 17:29:20	U	SMPL
L4272-04 - 1	MH-2-(6)	2736	0.5817	-	7471B	PPB	06 Oct 2020 17:31:37	U	SMPL
CCV66 - 1	CCV66	25985	5.2168	-	7471B	PPB	06 Oct 2020 17:33:53	U	SMPL
CCB66 - 1	CCB66	-158	0.0047	-	7471B	PPB	06 Oct 2020 17:36:08	U	SMPL
L4272-07 - 1	MH-3-(6)	3762	0.7862	-	7471B	PPB	06 Oct 2020 17:38:24	U	SMPL
L4272-10 - 1	GIS-1-(6)	4632	0.9597	-	7471B	PPB	06 Oct 2020 17:40:39	U	SMPL
L4272-13 - 1	GIS-2-(6)	651	0.1660	-	7471B	PPB	06 Oct 2020 17:42:54	U	SMPL
L4272-16 - 1	GIS-3-(6)	296	0.0952	-	7471B	PPB	06 Oct 2020 17:45:10	U	SMPL
L4272-19 - 1	GIS-4-(6)	205	0.0771	-	7471B	PPB	06 Oct 2020 17:47:25	U	SMPL
L4272-22 - 1	SC-1-(6.5)	2944	0.6231	-	7471B	PPB	06 Oct 2020 17:49:41	U	SMPL
L4272-25 - 1	SC-2-(6.5)	246	0.0852	-	7471B	PPB	06 Oct 2020 17:51:58	U	SMPL
L4272-28 - 1	SC-3-(6.5)	1160	0.2675	-	7471B	PPB	06 Oct 2020 17:54:15	U	SMPL
L4272-31 - 1	SC-4-(6.5)	774	0.1905	-	7471B	PPB	06 Oct 2020 17:56:32	U	SMPL
L4272-34 - 1	SC-5-(6.5)	561	0.1480	-	7471B	PPB	06 Oct 2020 17:58:48	U	SMPL
CCV67 - 1	CCV67	24498	4.9203	-	7471B	PPB	06 Oct 2020 18:01:03	U	SMPL
CCB67 - 1	CCB67	-200	-0.0037	-	7471B	PPB	06 Oct 2020 18:03:18	U	SMPL
L4272-37 - 1	SC-6-(6.5)	244	0.0848	-	7471B	PPB	06 Oct 2020 18:05:35	U	SMPL
L4272-40 - 1	SC-7-(6.5)	317	0.0994	-	7471B	PPB	06 Oct 2020 18:07:51	U	SMPL
L4272-43 - 1	SC-8-(6.5)	325	0.1010	-	7471B	PPB	06 Oct 2020 18:10:06	U	SMPL
L4272-46 - 1	SC-9-(3.5)	1536	0.3424	-	7471B	PPB	06 Oct 2020 18:12:22	U	SMPL
L4272-49 - 1	SC-10-(3.5)	2385	0.5117	-	7471B	PPB	06 Oct 2020 18:14:37	U	SMPL
L4272-52 - 1	SC-11-(3.5)	2575	0.5496	-	7471B	PPB	06 Oct 2020 18:16:54	U	SMPL
L4272-55 - 1	SC-12-(3.5)	979	0.2314	-	7471B	PPB	06 Oct 2020 18:19:10	U	SMPL
L4274-01 - 1	WC-1	353	0.1066	-	7471B	PPB	06 Oct 2020 18:21:27	U	SMPL
L4272-01LX5 - 1		362	0.1084	-	7471B	PPB	06 Oct 2020 18:23:44	U	SMPL
L4272-01A - 1		19830	3.9897	-	7471B	PPB	06 Oct 2020 18:25:59	U	SMPL
CCV68 - 1	CCV68	25684	5.1568	-	7471B	PPB	06 Oct 2020 18:28:15	U	SMPL
CCB68 - 1	CCB68	-142	0.0079	-	7471B	PPB	06 Oct 2020 18:30:31	U	SMPL